

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
 Data File : PD072035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 16:22
 Operator : AR\AJ
 Sample : PB147881BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS881

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/27/2022
 Supervised By : Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:23:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.829	3.563	42228367	579.9E6	16.656	18.822
27)	SA Decachlor...	8.019	9.092	85111615	333.8E6	36.304	37.263
Target Compounds							
2)	A alpha-BHC	3.338	4.029	16489508	216.6E6	4.452	5.091
3)	MA gamma-BHC...	3.670	4.364	15392756	188.8E6	4.402m	5.338m
4)	MA Heptachlor	4.016	4.942	15539853	147.8E6	4.374m	5.859 #
5)	MB Aldrin	4.301f	5.285	15642147	125.3E6	4.401	5.701 #
6)	B beta-BHC	3.968	4.570	7731056	77804276	4.830m	5.229m
7)	B delta-BHC	4.204f	4.819	13208271	126.6E6	3.730	5.081m#
8)	B Heptachlo...	4.806	5.715	14826897	96169795	4.657m	6.307m#
9)	A Endosulfan I	5.181	6.105	14202977	84915012	5.040	5.696
10)	B trans-Chl...	5.060	5.972	15366612	93008952	4.705	5.382
11)	B cis-Chlor...	5.125	6.049	15335434	91059455	4.779	5.410
12)	B 4,4'-DDE	5.315	6.223	26573919	163.6E6	8.979m	10.904
13)	MA Dieldrin	5.447	6.383	29533689	171.9E6	9.606m	11.383
14)	MA Endrin	5.725	6.616	25944920	131.7E6	9.786	10.682
15)	B Endosulfa...	6.019	6.841	24992026	138.3E6	10.014m	11.382
16)	A 4,4'-DDD	5.874	6.747	22440724	130.0E6	9.612	11.255
17)	MA 4,4'-DDT	6.128	7.058	22579086	129.2E6	9.424	11.357
18)	B Endrin al...	6.200	6.973	19727513	104.7E6	9.085m	10.100
19)	B Endosulfa...	6.424	7.205	23251751	116.1E6	9.214m	10.079
20)	A Methoxychlor	6.707	7.535	66618037	297.5E6	51.837	57.224
21)	B Endrin ke...	6.934	7.697	30408547	139.8E6	10.753m	11.194

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
Data File : PD072035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 16:22
Operator : AR\AJ
Sample : PB147881BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:23:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

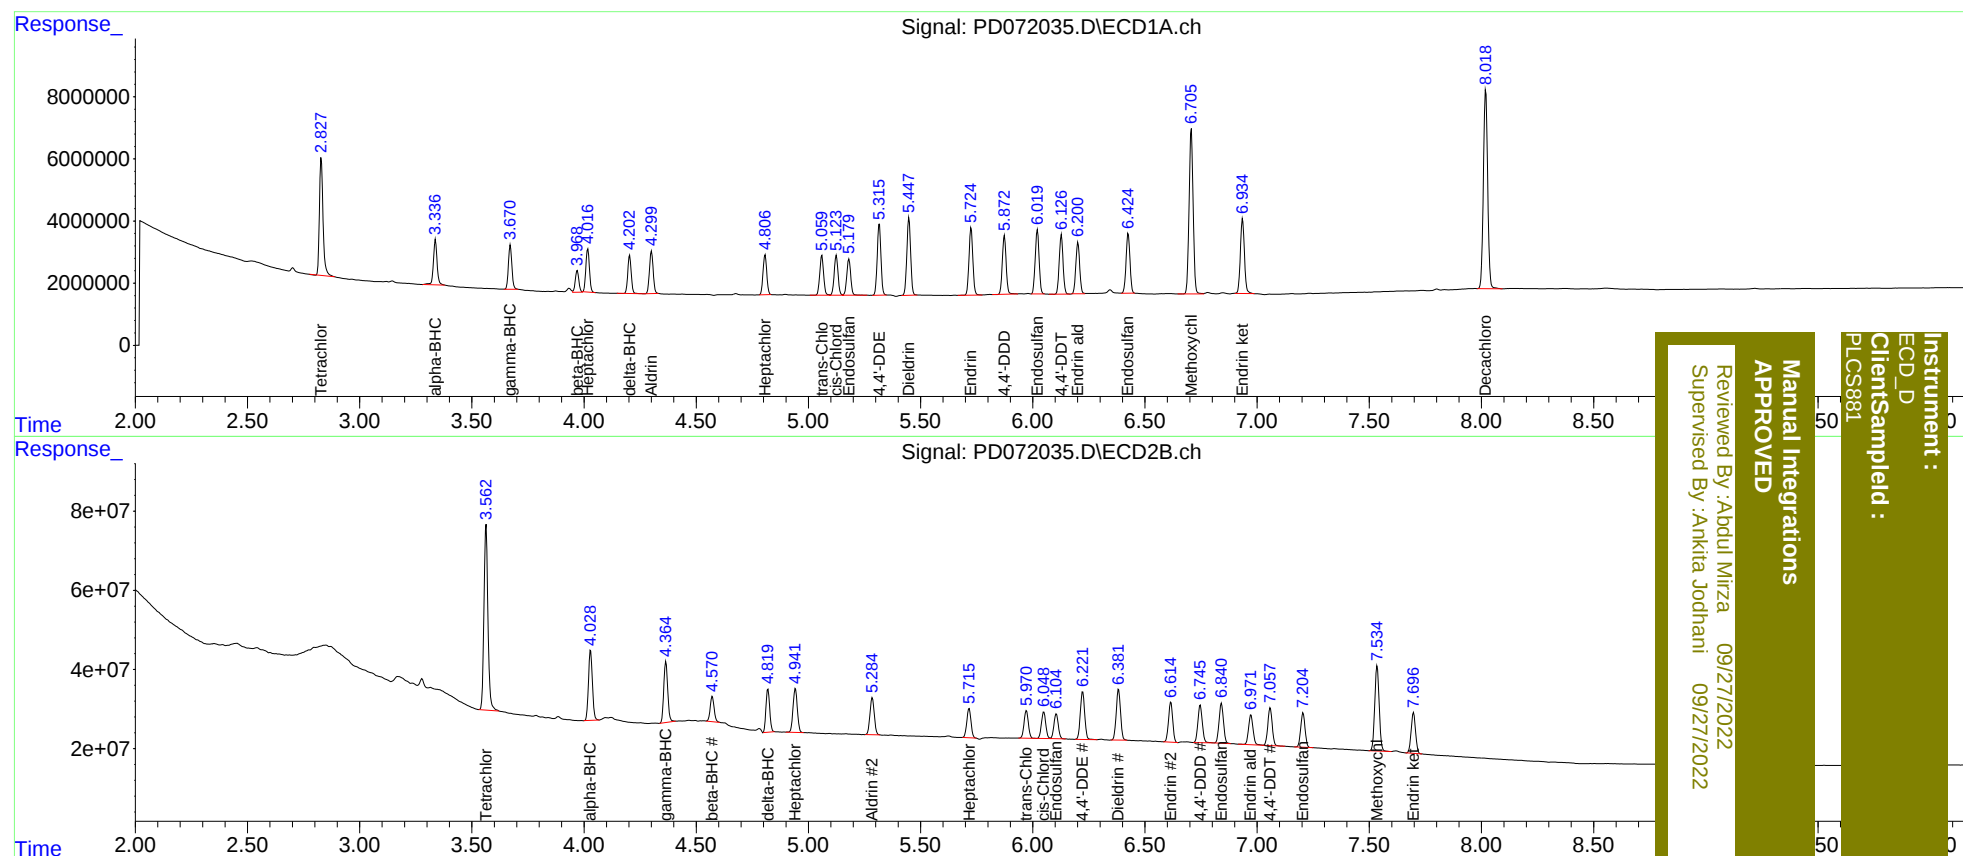

Reviewed By: Abdul Mirza 09/27/2022
Supervised By: Ankita Jodhani 09/27/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS881