

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
 Data File : PD055045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 14:47
 Operator : SG\AJ
 Sample : PIBLK42
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK42

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 22:59:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.298	3.961	16833530	23484147	22.127	22.885
27)	SA Decachlor...	7.978	8.999	33673015	44746800	39.964	38.407
Target Compounds							
2)	A alpha-BHC	3.750f	0.000	169257	0	0.152	N.D. #
9)	A Endosulfan I	5.233f	0.000	27010	0	<MDL	N.D. #
10)	B trans-Chl...	5.233f	0.000	27010	0	<MDL	N.D. #
11)	B cis-Chlor...	5.233	0.000	27010	0	<MDL	N.D. #
15)	B Endosulfa...	5.990f	0.000	2215998	0	2.544	N.D. #
16)	A 4,4'-DDD	5.990f	0.000	2215998	0	3.055	N.D. #
18)	B Endrin al...	6.281f	0.000	1352079	0	1.859	N.D. #
24)	Toxaphene-3	5.990	0.000	2215998	0	443.589	N.D. #
26)	Toxaphene-5	6.783	0.000	350222	0	18.933	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
Data File : PD055045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 14:47
Operator : SG\AJ
Sample : PIBLK42
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 22:59:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

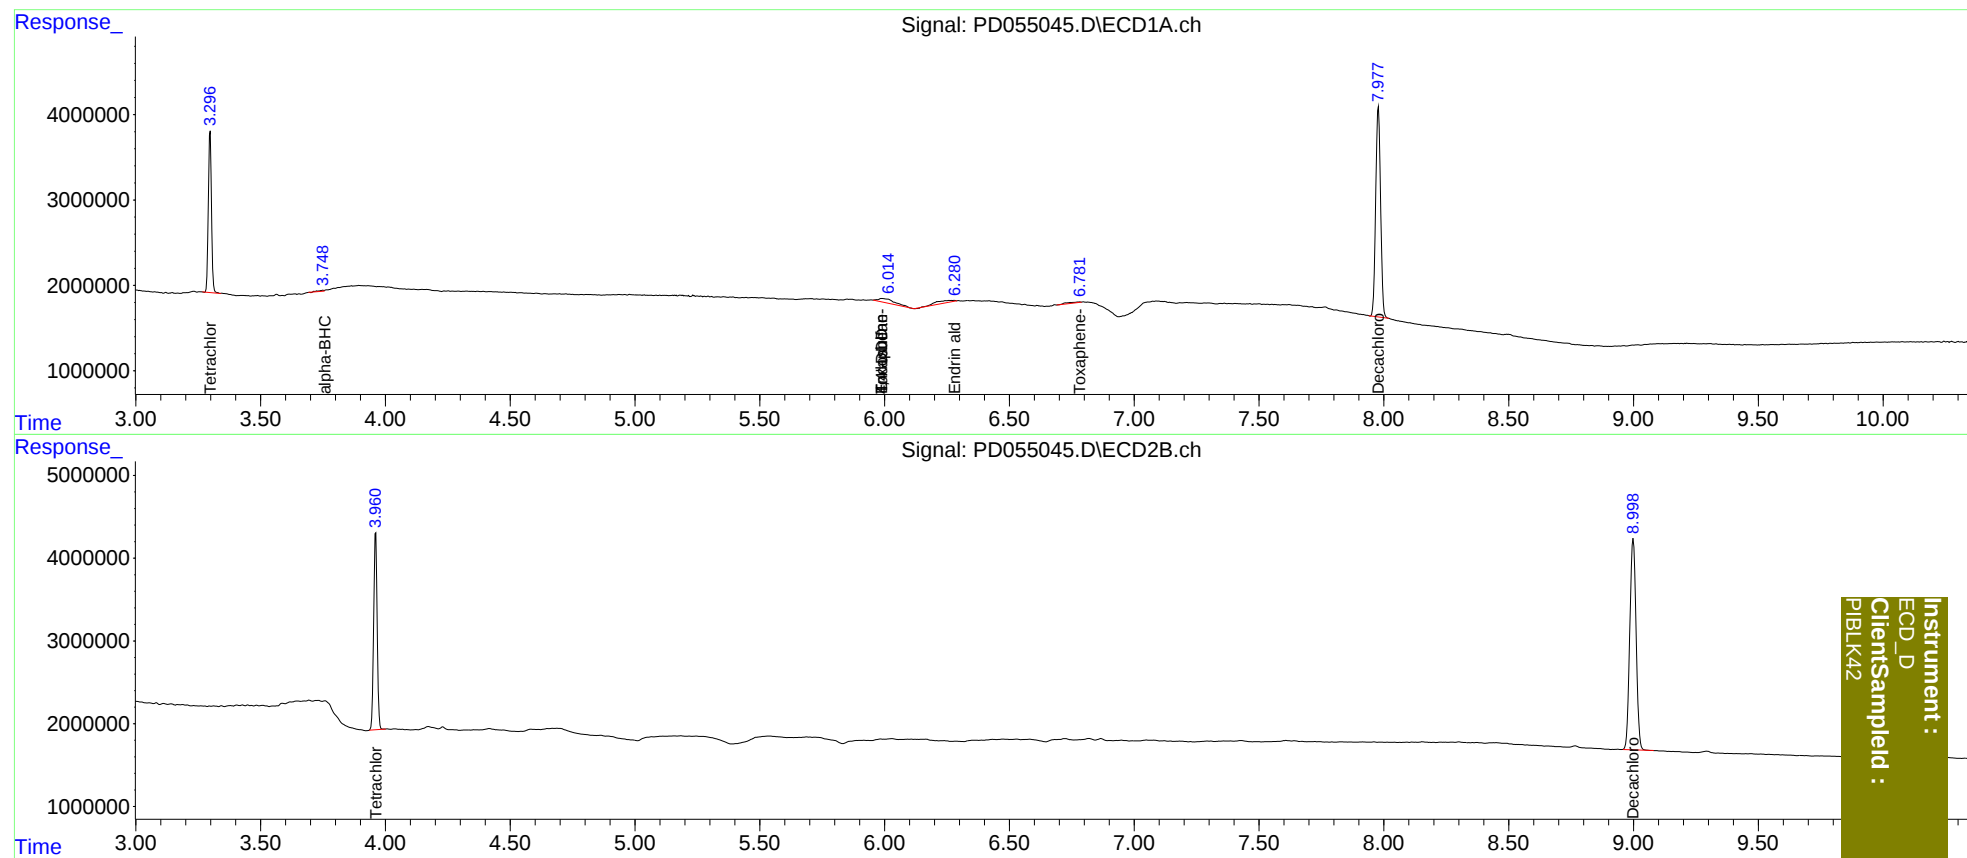


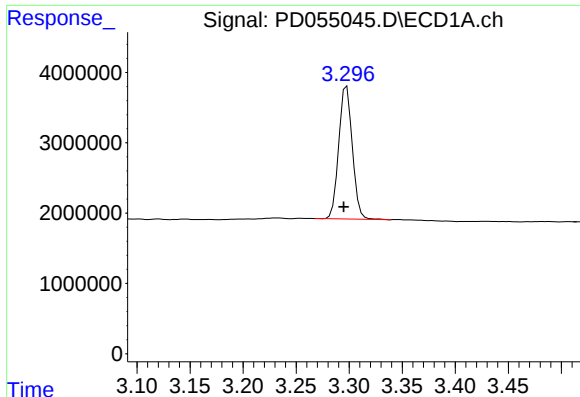

#1 Tetrachloro-m-xylene


R.T.: 3.298 min
Delta R.T.: 0.003 min
Response: 16833530
Conc: 22.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

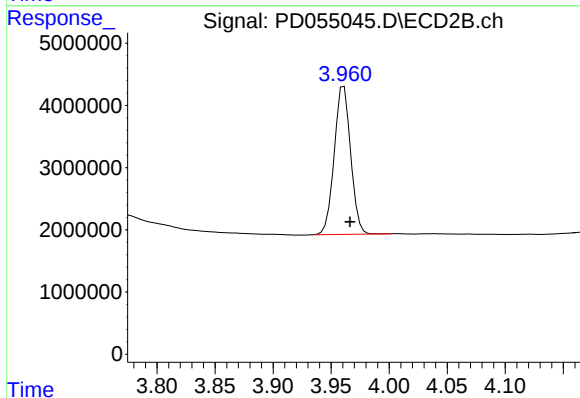


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.005 min
Response: 23484147
Conc: 22.88 ng/ml

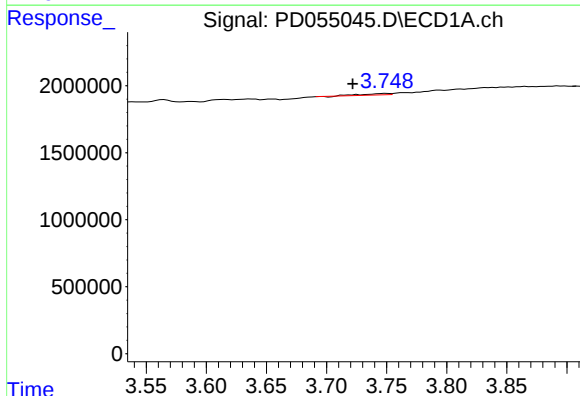


#2 alpha-BHC

R.T.: 3.750 min
Delta R.T.: 0.028 min
Response: 169257
Conc: 0.15 ng/ml

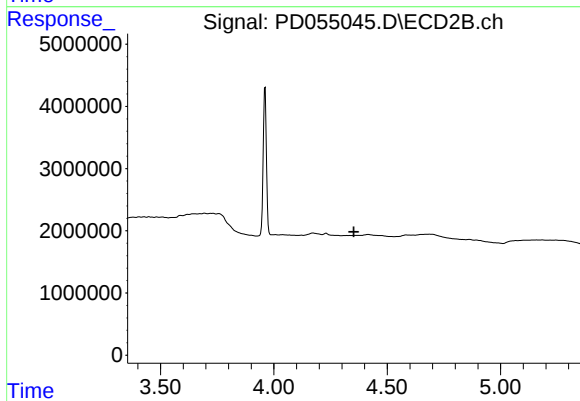

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.353 min
Response: 0
Conc: N.D.

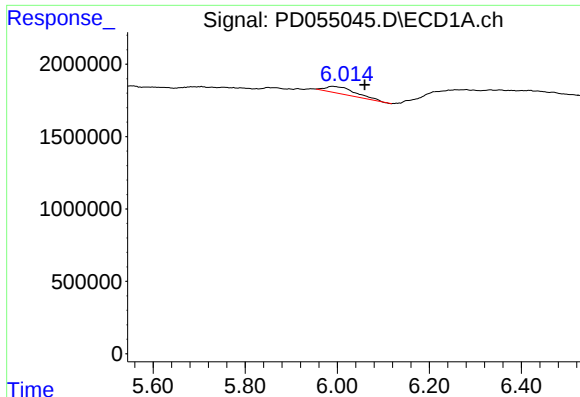

#15 Endosulfan II


R.T.: 5.990 min
Delta R.T.: -0.069 min
Response: 2215998
Conc: 2.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

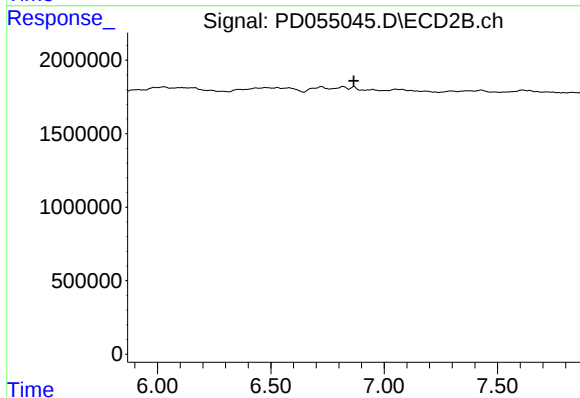


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.866 min
Response: 0
Conc: N.D.

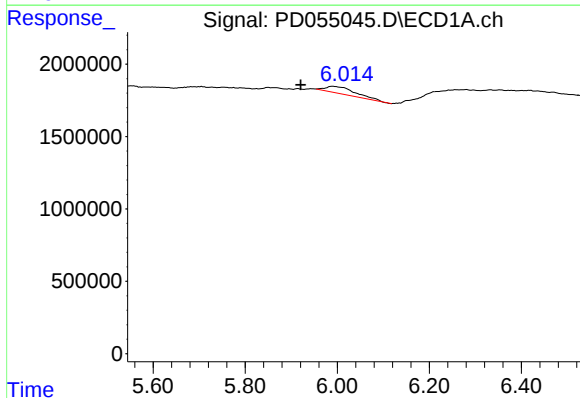


#16 4,4'-DDD

R.T.: 5.990 min
Delta R.T.: 0.070 min
Response: 2215998
Conc: 3.06 ng/ml

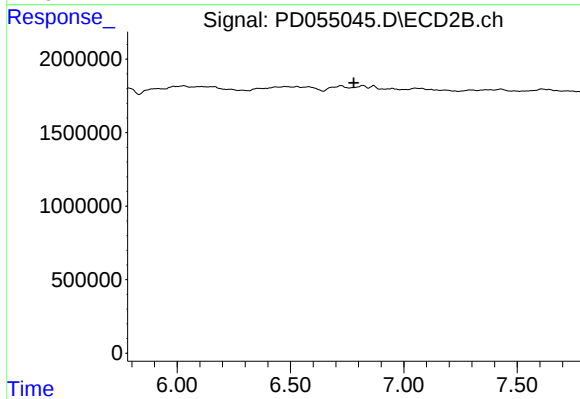

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

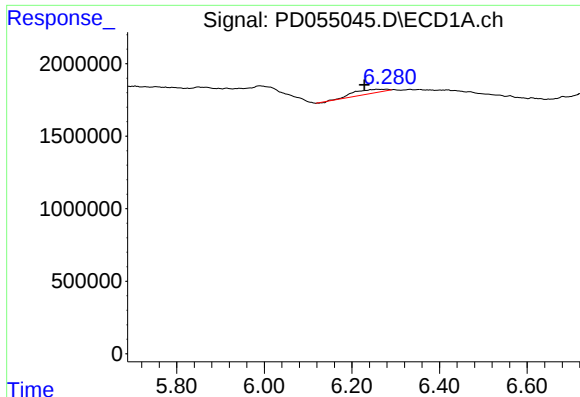

#18 Endrin aldehyde


R.T.: 6.281 min
Delta R.T.: 0.053 min
Response: 1352079
Conc: 1.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

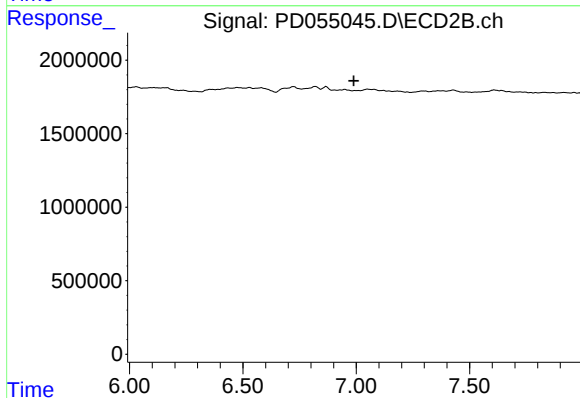


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

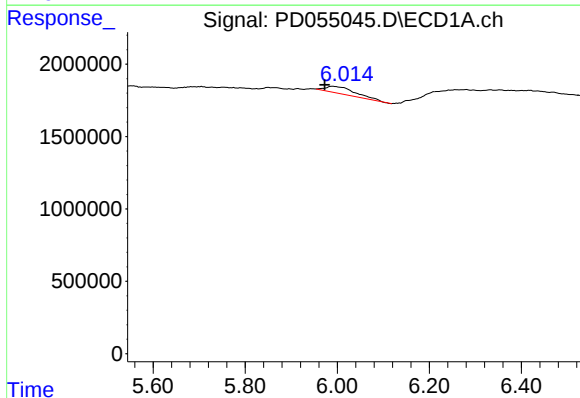


#24 Toxaphene-3

R.T.: 5.990 min
Delta R.T.: 0.018 min
Response: 2215998
Conc: 443.59 ng/ml

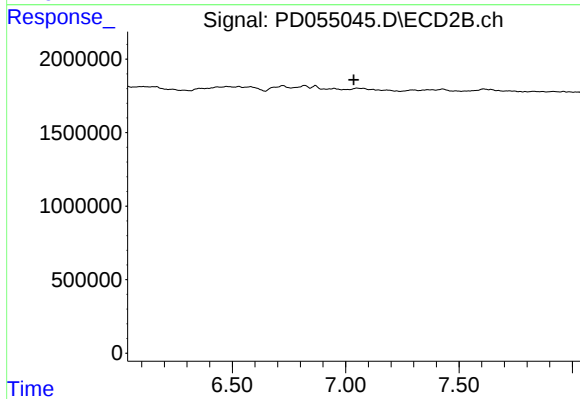

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T. : 7.036 min
Response: 0
Conc: N.D.

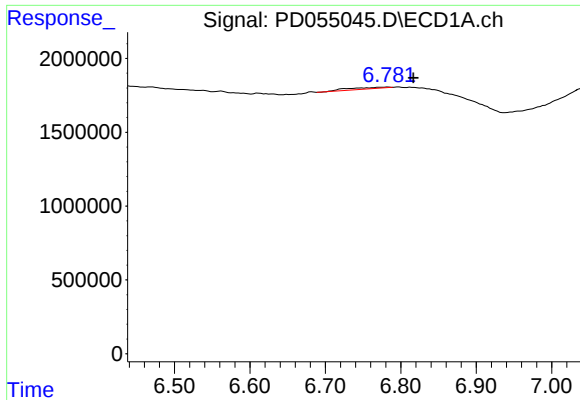

#26 Toxaphene-5


R.T.: 6.783 min
Delta R.T.: -0.034 min
Response: 350222
Conc: 18.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

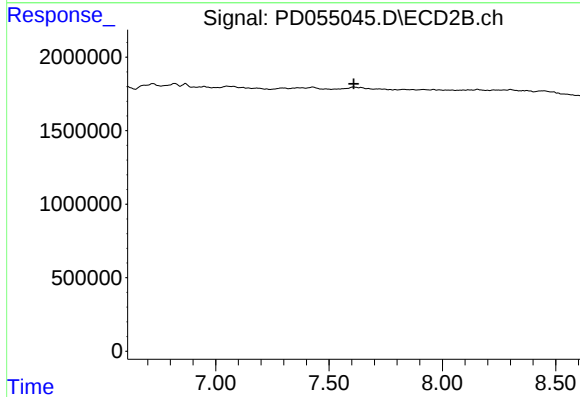


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.610 min
Response: 0
Conc: N.D.

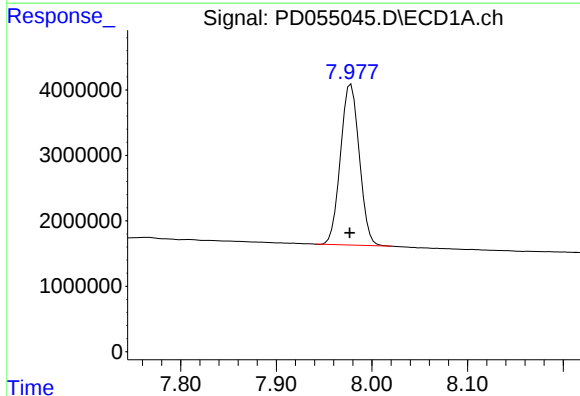

#27 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: 0.001 min
Response: 33673015
Conc: 39.96 ng/ml

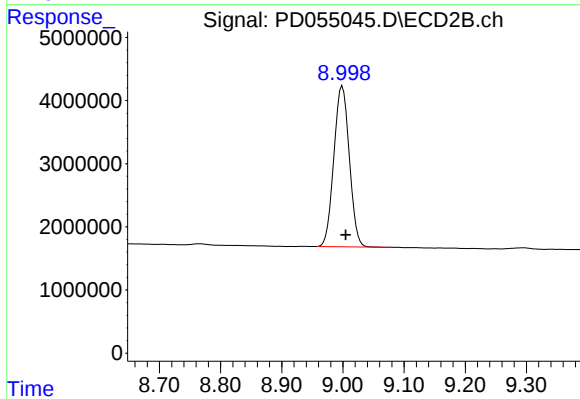

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.006 min
Response: 44746800
Conc: 38.41 ng/ml