

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
 Data File : PD055030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 10:10
 Operator : SG\AJ
 Sample : MDL-TOX-S-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-TOX-S-02

Manual Integrations
 APPROVED

Ankita
 9/30/2019 11:22:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 11:00:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	15468980	21720131	20.333	21.166
27)	SA Decachlor...	7.970	8.997	29986121	39786590	35.588	34.150
Target Compounds							
22)	Toxaphene-1	5.492	6.336	682496	828321	122.000	126.090m
23)	Toxaphene-2	5.646	6.624	484645	809358	83.623	95.760m
24)	Toxaphene-3	5.969	7.029	529610	1033601	106.015	84.309m
25)	Toxaphene-4	6.085	7.105	1303509	2966857	86.185	88.095
26)	Toxaphene-5	6.809	7.604	1601663	1398131	86.585m	85.162

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
Data File : PD055030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 10:10
Operator : SG\AJ
Sample : MDL-TOX-S-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 11:00:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

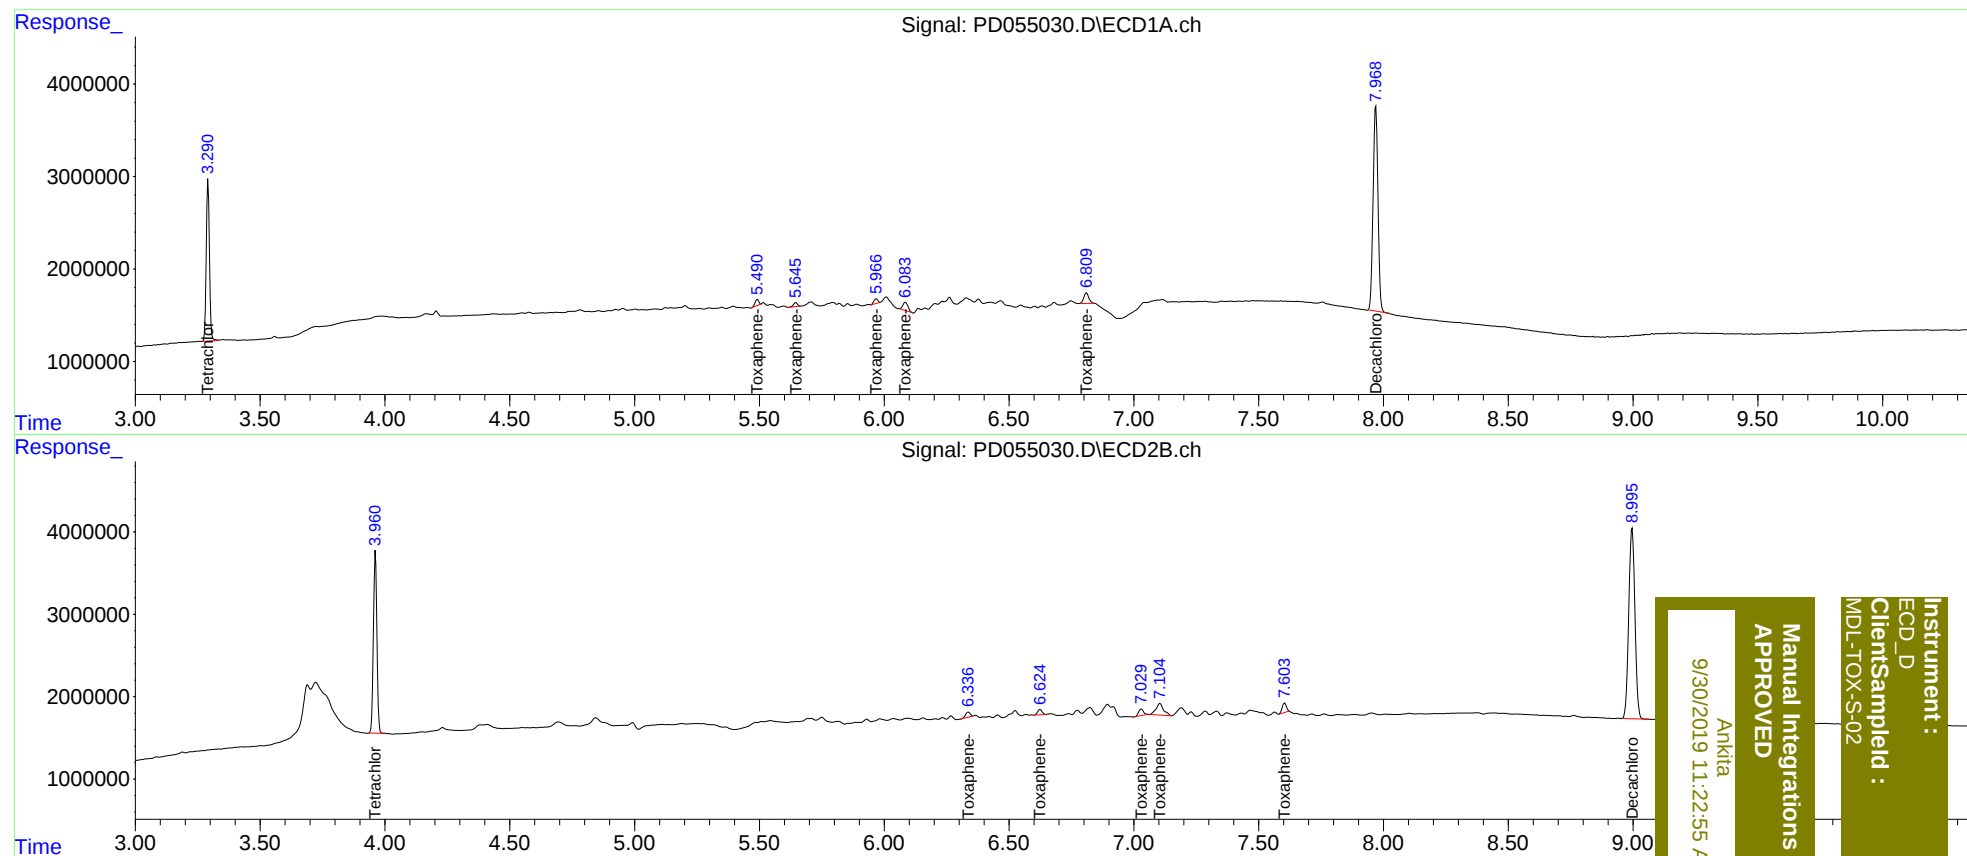

Manual Integrations
APPROVED

Ankita

9/30/2019 11:22:55 AM

Instrument :
ECD_D
Client Sampled :
MDL-TOX-S-02