

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
 Data File : PD055031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 10:25
 Operator : SG\AJ
 Sample : MDL-TOX-S-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-TOX-S-03

Manual Integrations
 APPROVED

Ankita
 9/30/2019 11:22:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 11:00:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	16348812	22860295	21.490	22.277
27)	SA Decachlor...	7.970	8.996	31537229	41921657	37.429	35.982
Target Compounds							
22)	Toxaphene-1	5.492	6.335	770956	836432	137.812	127.325m
23)	Toxaphene-2	5.648	6.623	596268	855886	102.883	101.266m
24)	Toxaphene-3	5.968	7.029	622936	1225612	124.697	99.970m
25)	Toxaphene-4	6.084	7.106	1453406	3286389	96.096	97.583
26)	Toxaphene-5	6.810	7.604	1762764	1498784	95.294m	91.293

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
Data File : PD055031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 10:25
Operator : SG\AJ
Sample : MDL-TOX-S-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 11:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

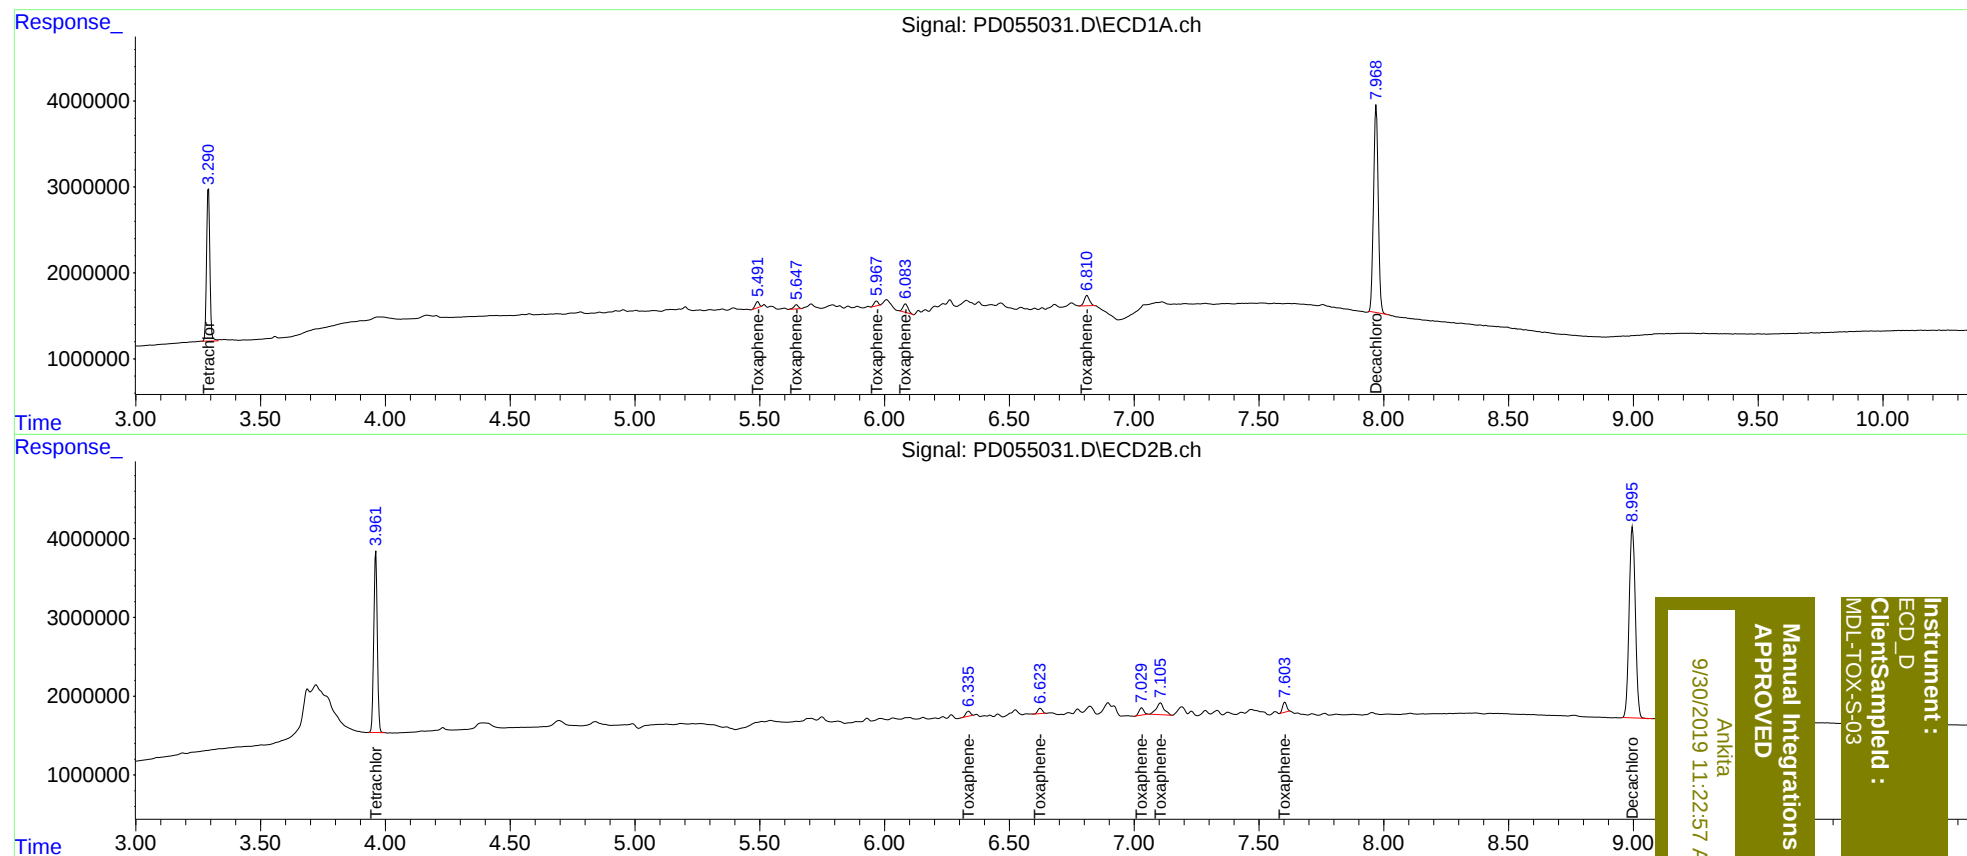

Manual Integrations
APPROVED

Ankita
9/30/2019 11:22:57 AM

Instrument :
ECD_D
ClientSample :
MDL-TOX-S-03