

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
 Data File : PD055032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 10:39
 Operator : SG\AJ
 Sample : MDL-TOX-S-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-TOX-S-04

Manual Integrations
 APPROVED

Ankita
 9/30/2019 11:22:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 11:00:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	17560988	24540120	23.083	23.914
27)	SA Decachlor...	7.969	8.997	33395158	45198758	39.634	38.795
Target Compounds							
22)	Toxaphene-1	5.492	6.336	803238	856978	143.583	130.452m
23)	Toxaphene-2	5.647	6.623	579874	938064	100.055	110.989m
24)	Toxaphene-3	5.967	7.030	616707	1118238	123.450	91.212 #
25)	Toxaphene-4	6.085	7.107	1454945	3406513	96.198	101.150
26)	Toxaphene-5	6.809	7.604	1891407	1634931	102.249m	99.586

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092719\
Data File : PD055032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 10:39
Operator : SG\AJ
Sample : MDL-TOX-S-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 11:00:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

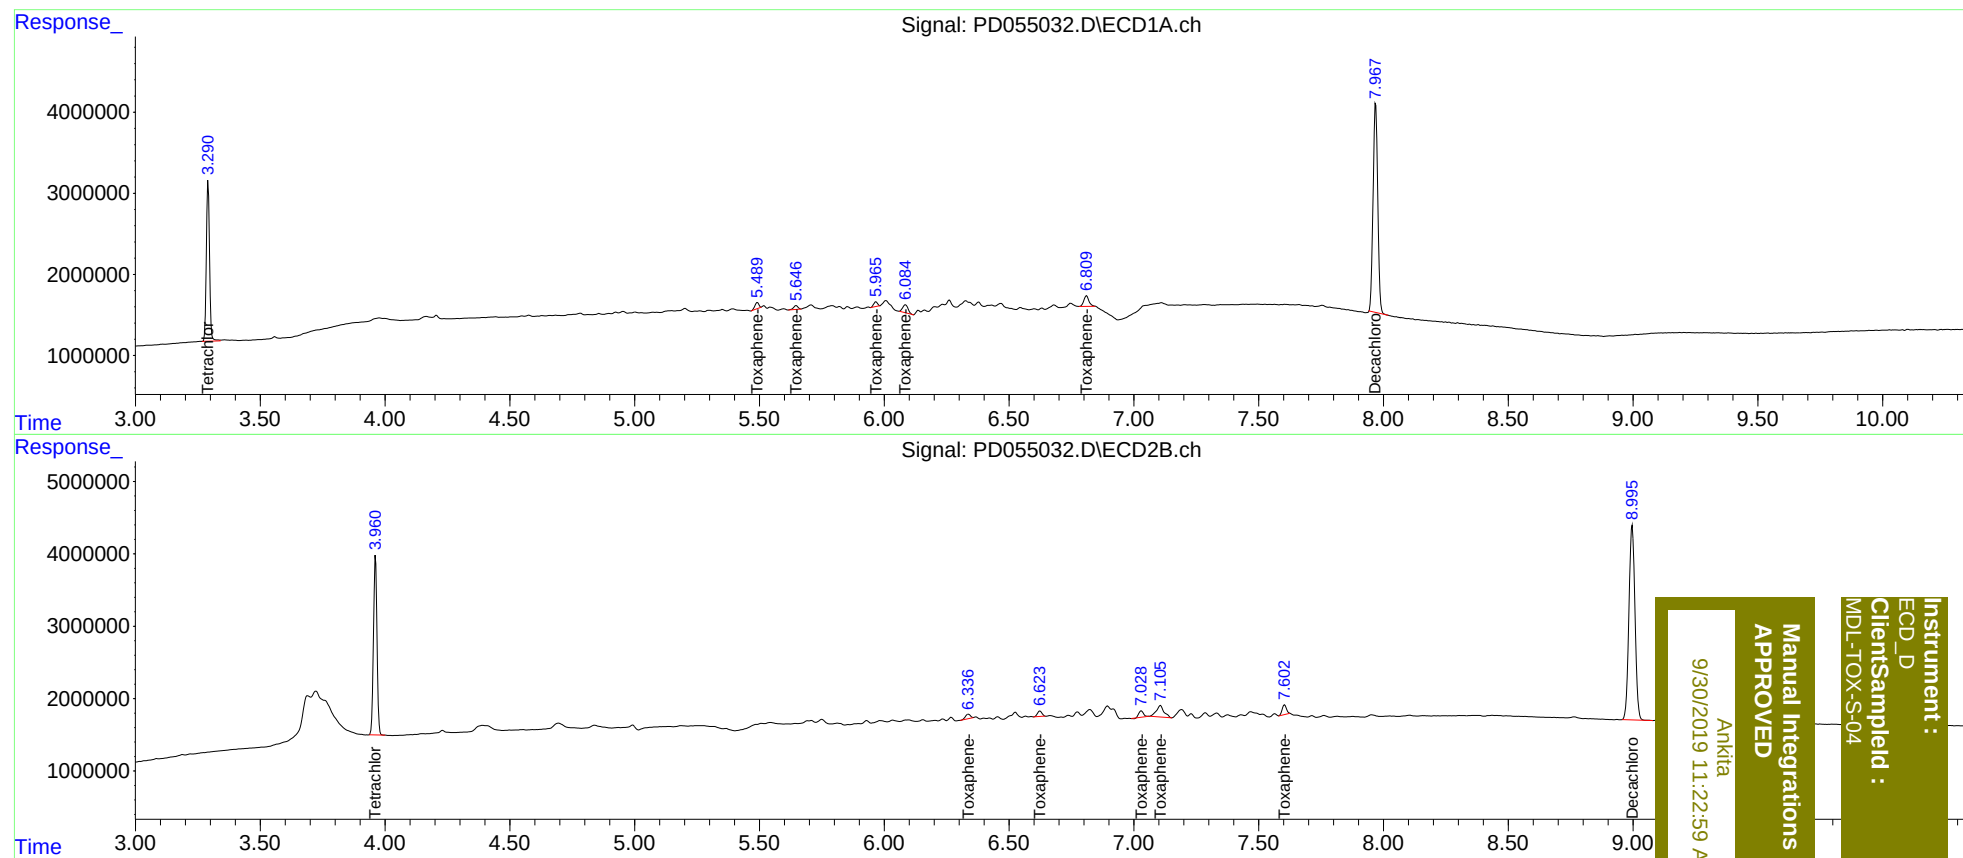

Manual Integrations
APPROVED

Ankita

9/30/2019 11:22:59 AM

Instrument :
ECD_D
Client Sampled :
MDL-TOX-S-04