

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
 Data File : PD065919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2021 20:21
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:56:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.013	38988840	292.0E6	52.648	50.847
2)	SA Decachlor...	8.236	9.087	59612287	186.5E6	43.642	48.198
Target Compounds							
2)	A alpha-BHC	3.932	4.408	60547361	425.6E6	53.912	50.617
3)	MA gamma-BHC...	4.216	4.694	58973760	393.4E6	52.590	50.916
4)	MA Heptachlor	4.513	5.198	61826894	355.2E6	51.833	48.955
5)	MB Aldrin	4.761	5.503	60470350	335.4E6	54.055	49.849
6)	B beta-BHC	4.464	4.871	29743635	180.8E6	52.102	48.923
7)	B delta-BHC	4.669	5.088	61463700	378.0E6	54.370	52.518
8)	B Heptachlo...	5.204	5.893	60088323	302.5E6	53.663	58.532
9)	A Endosulfan I	5.542	6.251	57563049	286.3E6	52.930	51.798
10)	B gamma-Chl...	5.428	6.127	62242222	305.6E6	51.545	50.955
11)	B alpha-Chl...	5.487	6.199	61875605	300.4E6	52.270	50.044
12)	B 4,4'-DDE	5.649	6.357	57788844	294.6E6	53.090	51.081
13)	MA Dieldrin	5.785	6.509	61668743	304.7E6	53.207	51.704
14)	MA Endrin	6.043	6.729	50002578	231.6E6	47.255	46.980
15)	B Endosulfa...	6.315	6.942	55507086	251.9E6	51.381	52.008
16)	A 4,4'-DDD	6.164	6.852	53228880	255.3E6	54.263	51.945
17)	MA 4,4'-DDT	6.405	7.149	54247306	243.5E6	49.284	48.206
18)	B Endrin al...	6.484	7.066	45386499	202.5E6	51.211	51.723
19)	B Endosulfa...	6.695	7.289	59840281	252.5E6	52.429	51.195
20)	A Methoxychlor	6.951	7.609	32934764	128.8E6	48.195	48.939
21)	B Endrin ke...	7.189	7.763	75763993	297.3E6	53.785	52.134
22)	Mirex	7.374	8.212	58140028	193.2E6	48.154	48.926



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
Data File : PD065919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2021 20:21
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:56:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

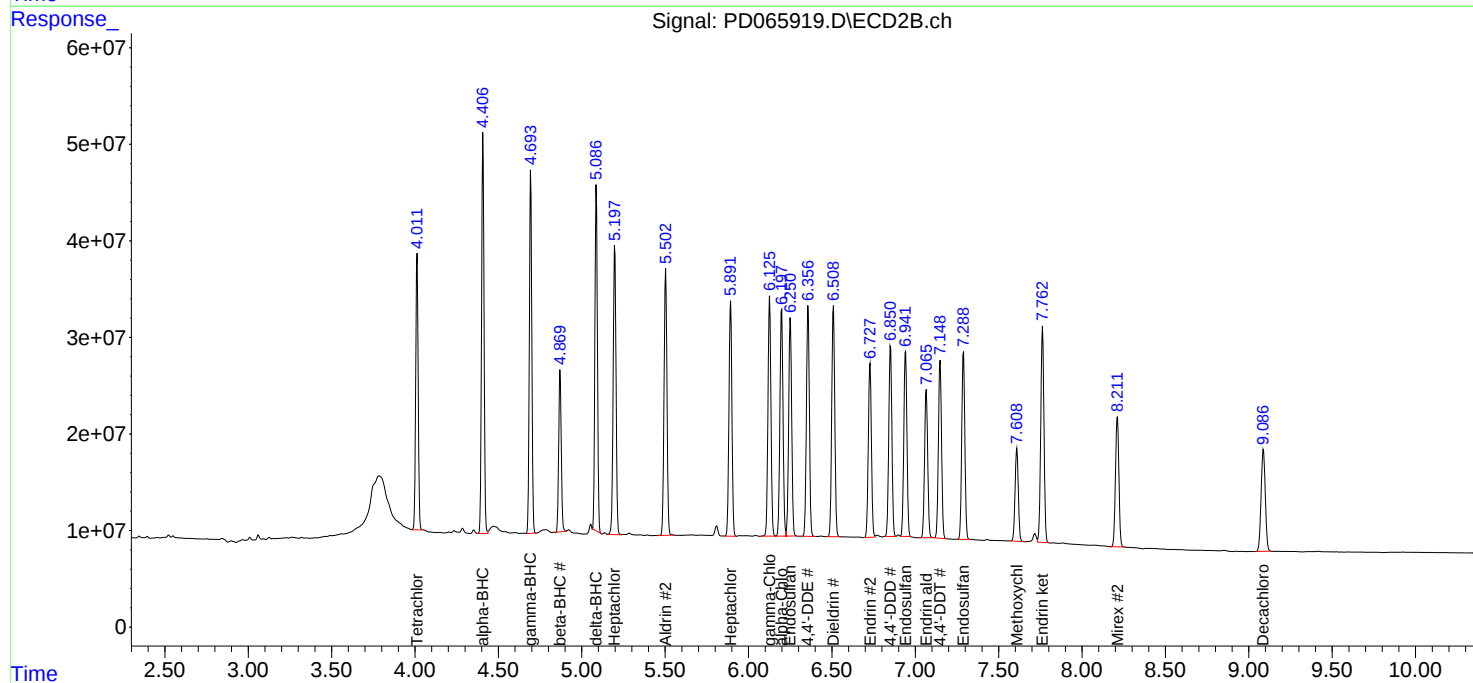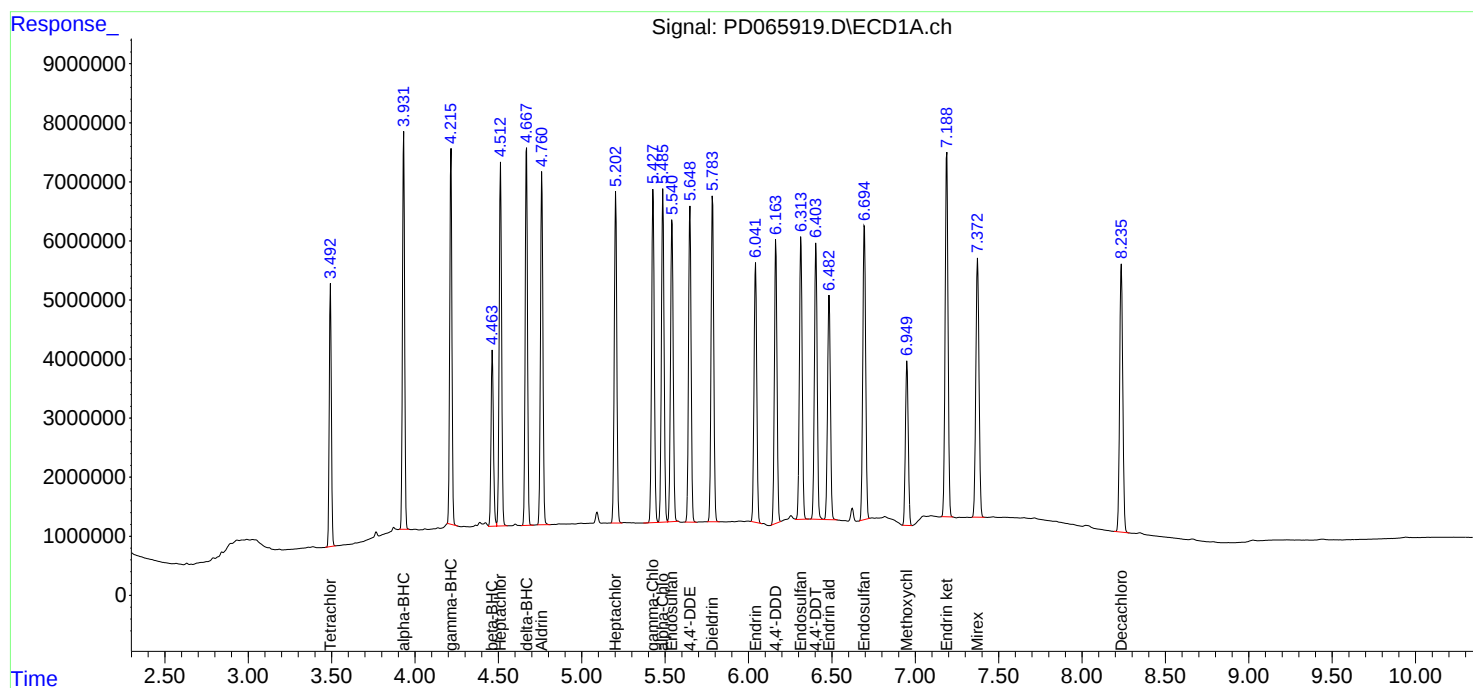


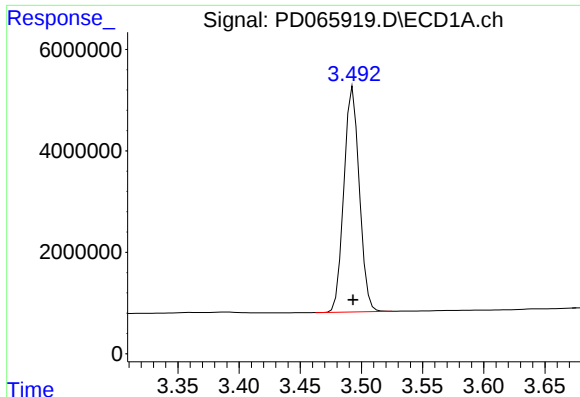

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 38988840
Conc: 52.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

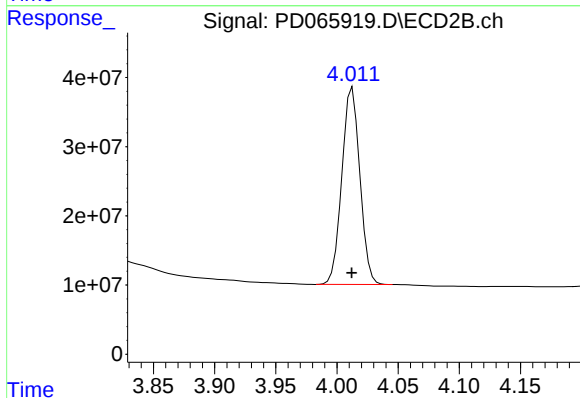


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 291971687
Conc: 50.85 ng/ml

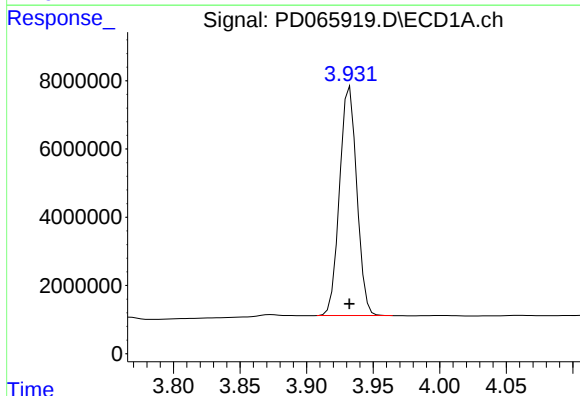


#2 alpha-BHC

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 60547361
Conc: 53.91 ng/ml

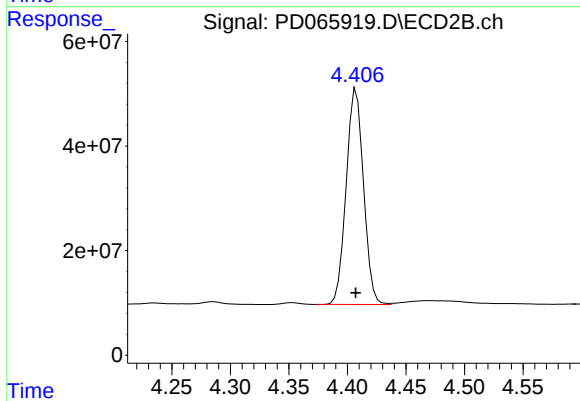

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 425595100
Conc: 50.62 ng/ml

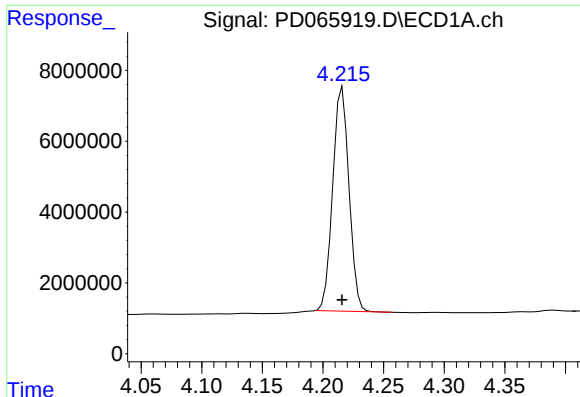

#3 gamma-BHC (Lindane)


R.T.: 4.216 min
Delta R.T.: 0.000 min
Response: 58973760
Conc: 52.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

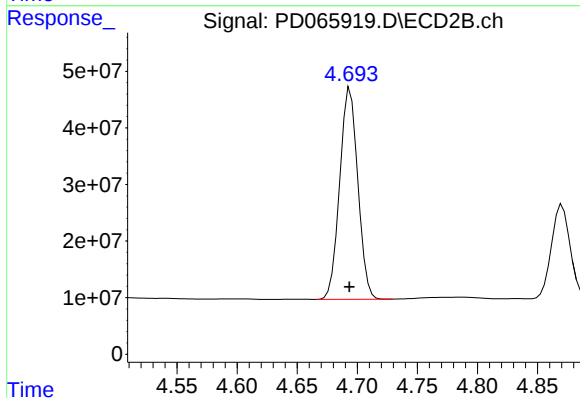


#3 gamma-BHC (Lindane)

R.T.: 4.694 min
Delta R.T.: 0.000 min
Response: 393369655
Conc: 50.92 ng/ml

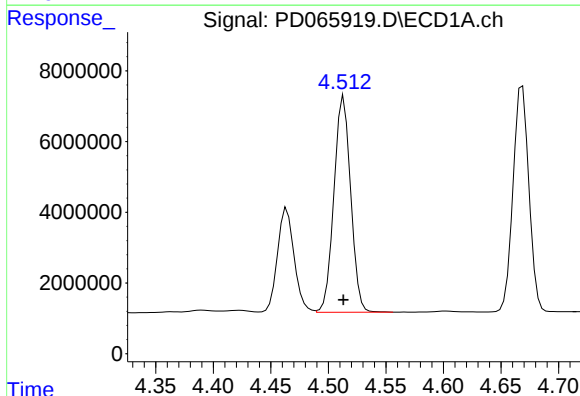


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 61826894
Conc: 51.83 ng/ml

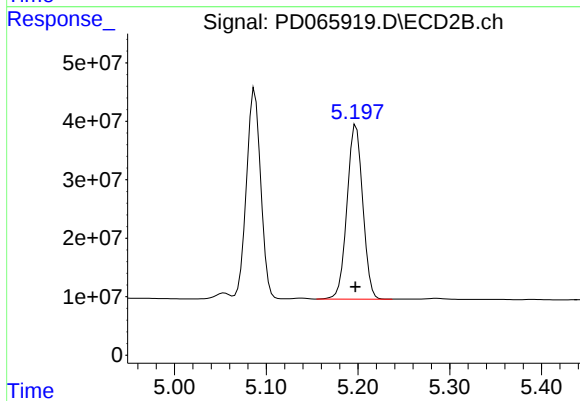

#4 Heptachlor


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 355205240
Conc: 48.95 ng/ml

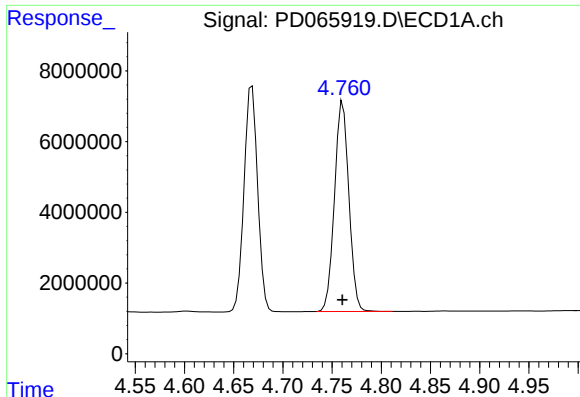

#5 Aldrin


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 60470350
Conc: 54.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

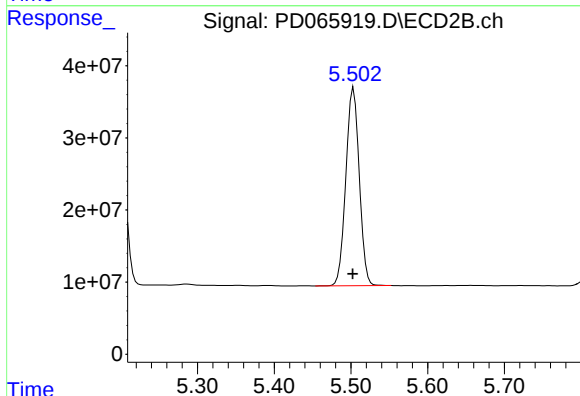


#5 Aldrin

R.T.: 5.503 min
Delta R.T.: 0.001 min
Response: 335361417
Conc: 49.85 ng/ml

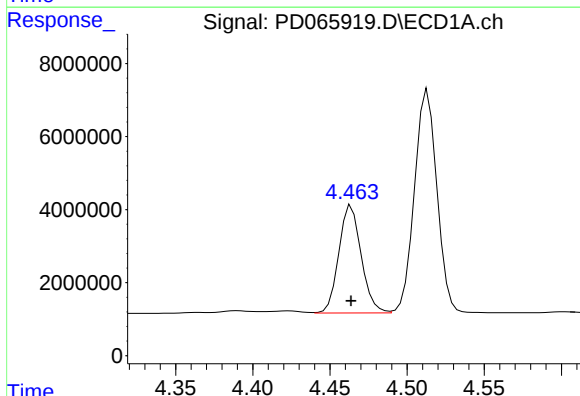


#6 beta-BHC

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 29743635
Conc: 52.10 ng/ml

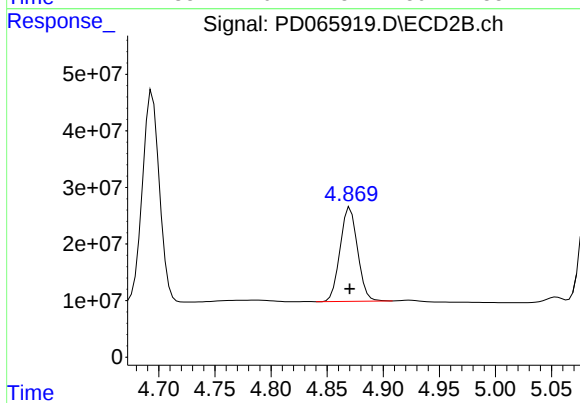

#6 beta-BHC


R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 180813948
Conc: 48.92 ng/ml

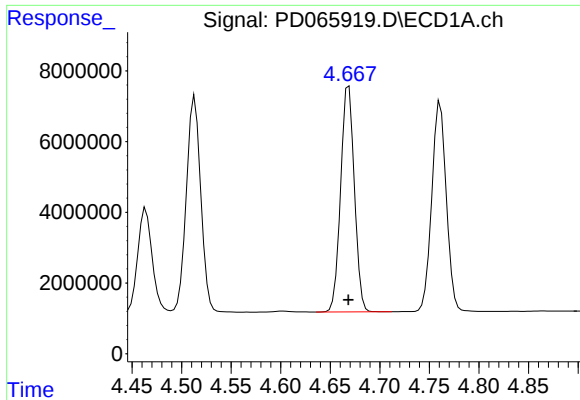

#7 delta-BHC


R.T.: 4.669 min
Delta R.T.: 0.000 min
Response: 61463700
Conc: 54.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

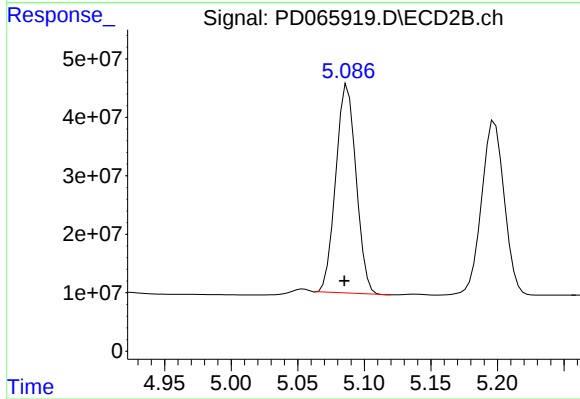


#7 delta-BHC

R.T.: 5.088 min
Delta R.T.: 0.002 min
Response: 377956766
Conc: 52.52 ng/ml

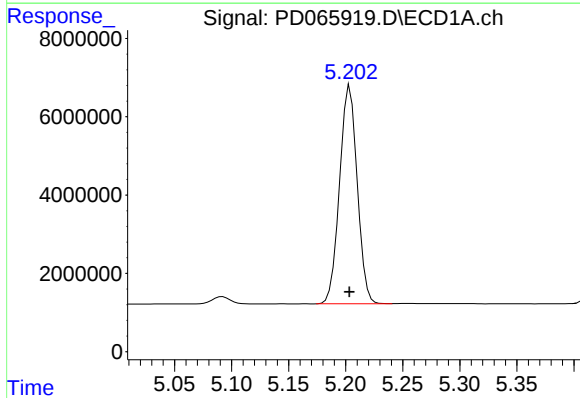


#8 Heptachlor epoxide

R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 60088323
Conc: 53.66 ng/ml

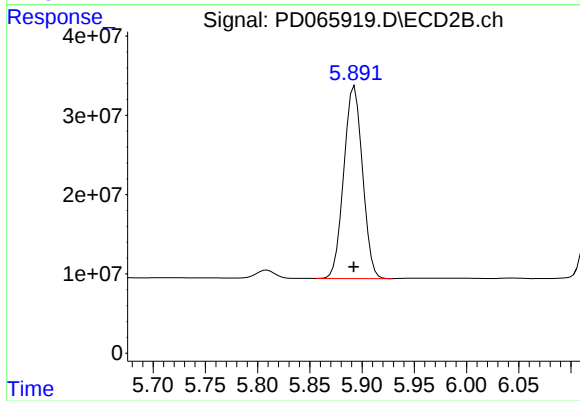

#8 Heptachlor epoxide


R.T.: 5.893 min
Delta R.T.: 0.000 min
Response: 302486444
Conc: 58.53 ng/ml

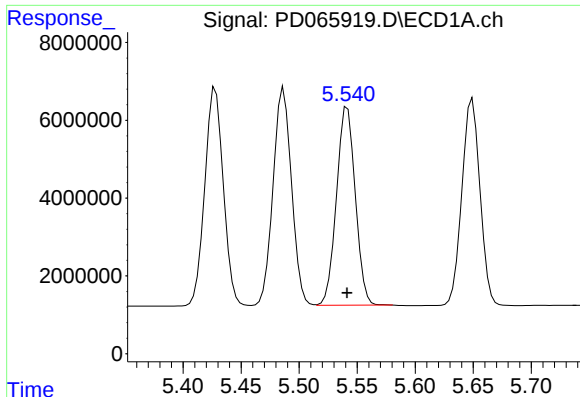

#9 Endosulfan I


R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 57563049
Conc: 52.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

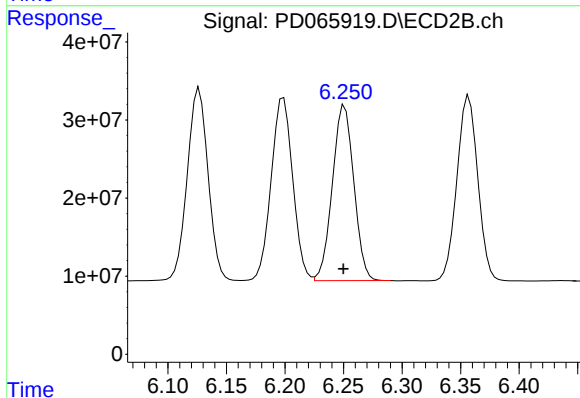


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: 0.001 min
Response: 286288591
Conc: 51.80 ng/ml

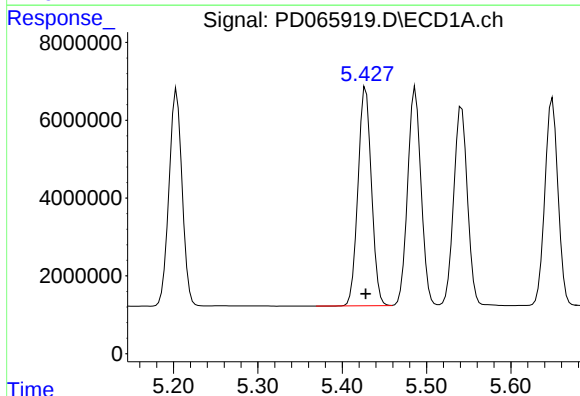


#10 gamma-Chlordane

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 62242222
Conc: 51.54 ng/ml

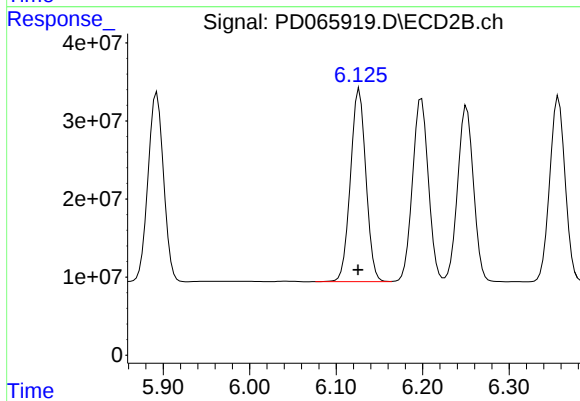

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.001 min
Response: 305612855
Conc: 50.95 ng/ml

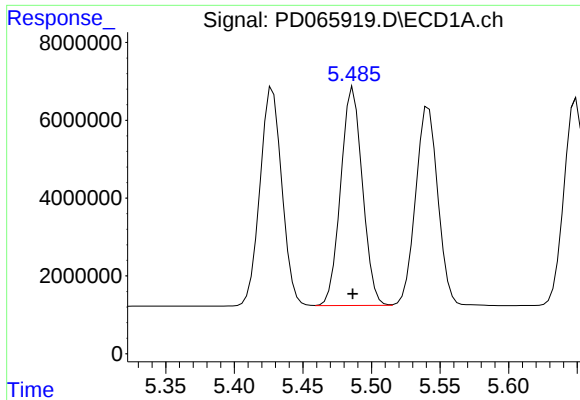

#11 alpha-Chlordane


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 61875605
Conc: 52.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

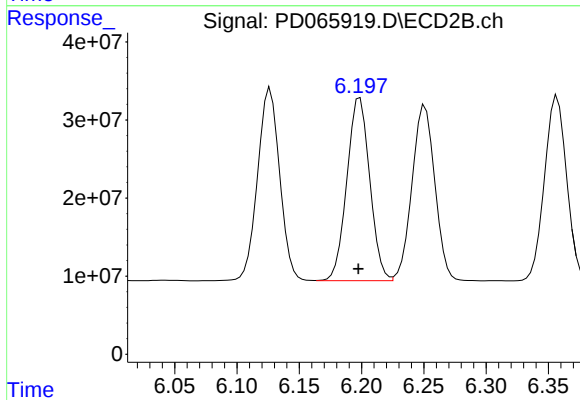


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 300367633
Conc: 50.04 ng/ml

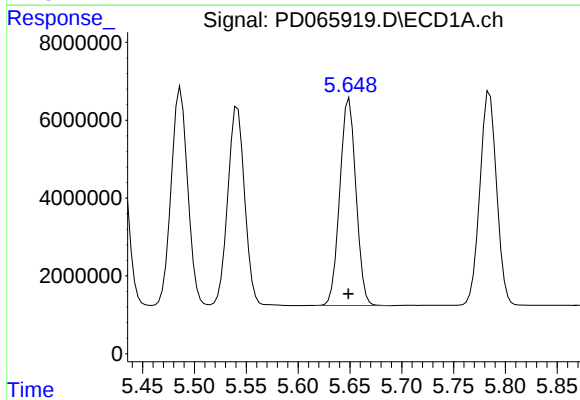


#12 4,4'-DDE

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 57788844
Conc: 53.09 ng/ml

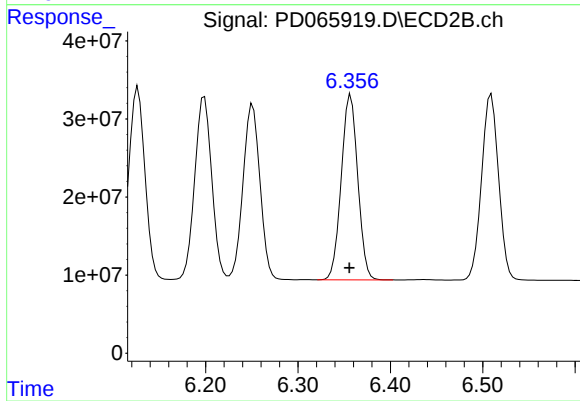

#12 4,4'-DDE


R.T.: 6.357 min
Delta R.T.: 0.001 min
Response: 294605284
Conc: 51.08 ng/ml

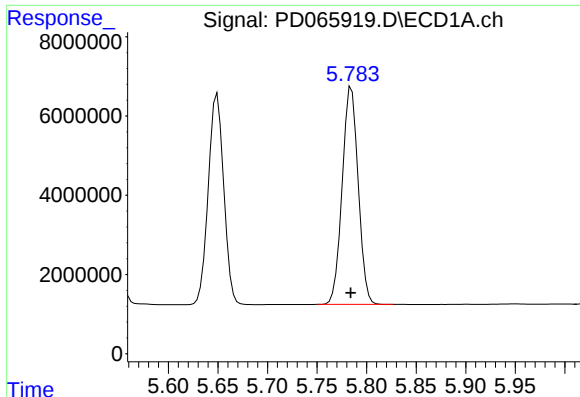

#13 Dieldrin


R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 61668743
Conc: 53.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

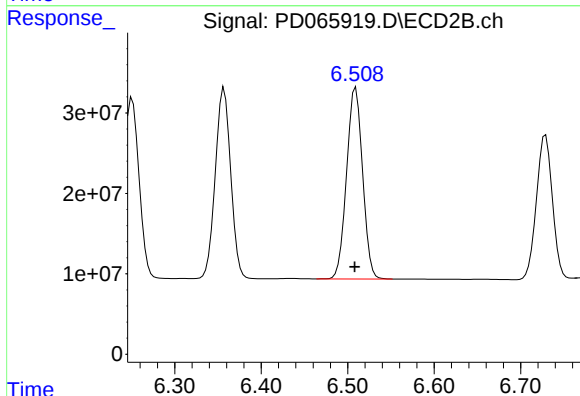


#13 Dieldrin

R.T.: 6.509 min
Delta R.T.: 0.001 min
Response: 304702181
Conc: 51.70 ng/ml

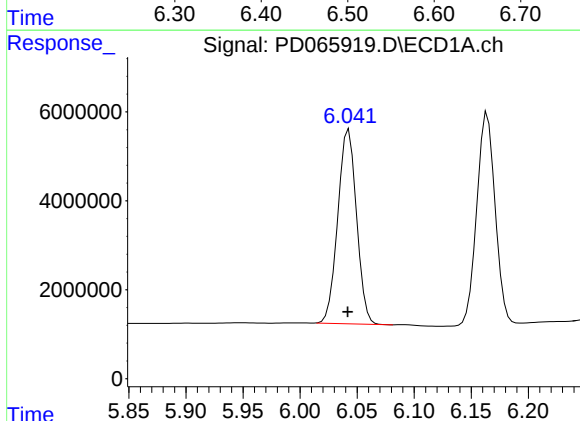


#14 Endrin

R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 50002578
Conc: 47.25 ng/ml

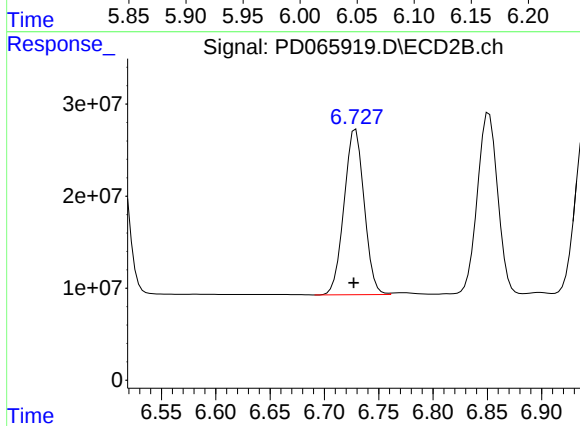

#14 Endrin


R.T.: 6.729 min
Delta R.T.: 0.002 min
Response: 231615434
Conc: 46.98 ng/ml

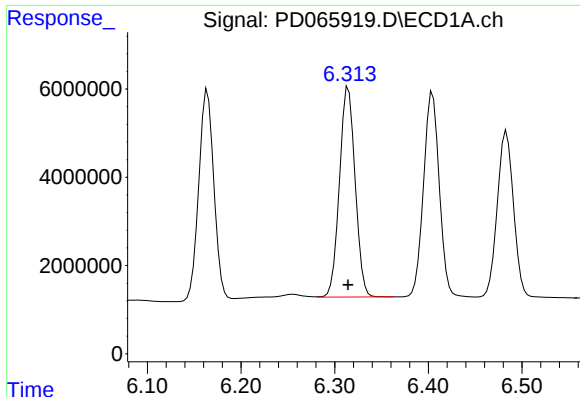

#15 Endosulfan II


R.T.: 6.315 min
Delta R.T.: 0.000 min
Response: 55507086
Conc: 51.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

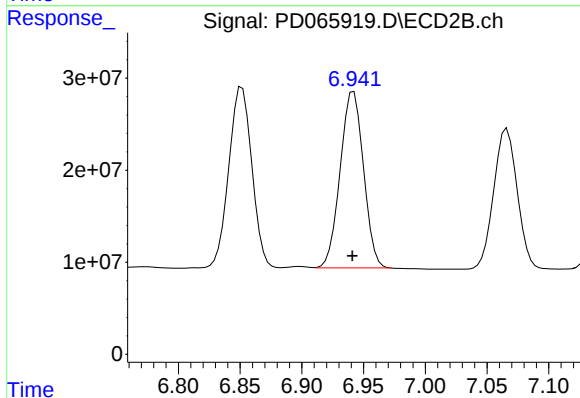


#15 Endosulfan II

R.T.: 6.942 min
Delta R.T.: 0.001 min
Response: 251918810
Conc: 52.01 ng/ml

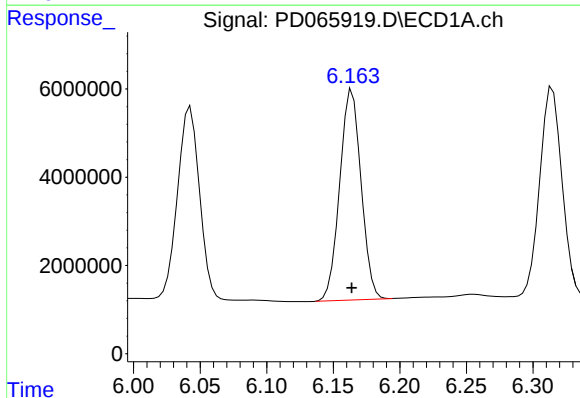


#16 4,4'-DDD

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 53228880
Conc: 54.26 ng/ml

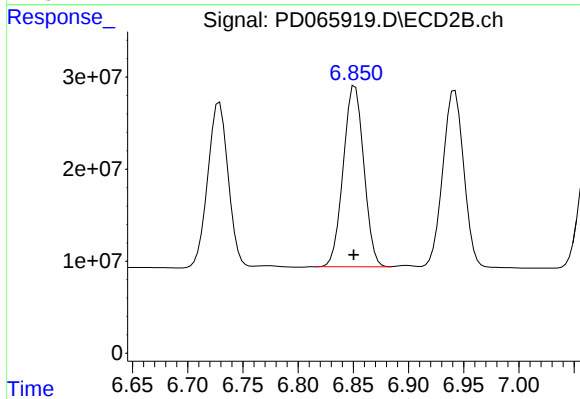

#16 4,4'-DDD


R.T.: 6.852 min
Delta R.T.: 0.001 min
Response: 255287604
Conc: 51.95 ng/ml

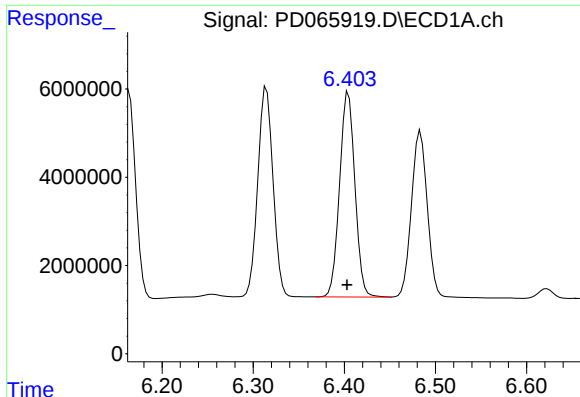

#17 4,4'-DDT


R.T.: 6.405 min
Delta R.T.: 0.002 min
Response: 54247306
Conc: 49.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

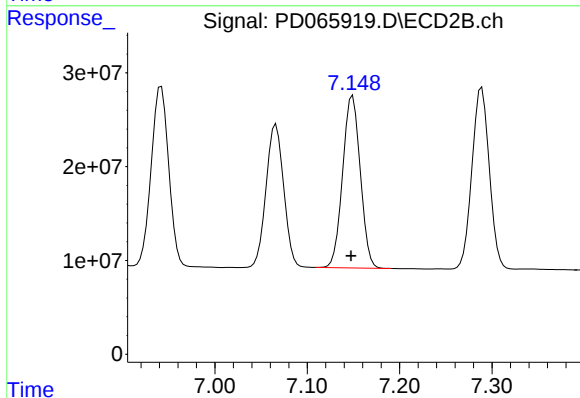


#17 4,4'-DDT

R.T.: 7.149 min
Delta R.T.: 0.002 min
Response: 243508812
Conc: 48.21 ng/ml

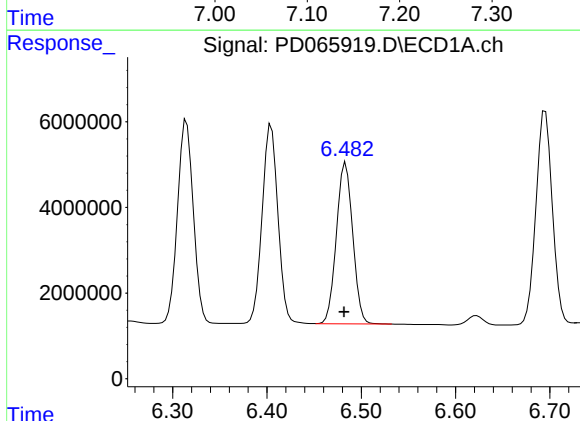


#18 Endrin aldehyde

R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 45386499
Conc: 51.21 ng/ml

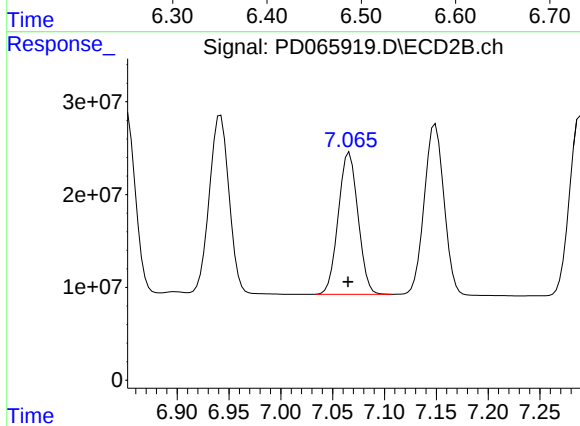

#18 Endrin aldehyde


R.T.: 7.066 min
Delta R.T.: 0.001 min
Response: 202493191
Conc: 51.72 ng/ml

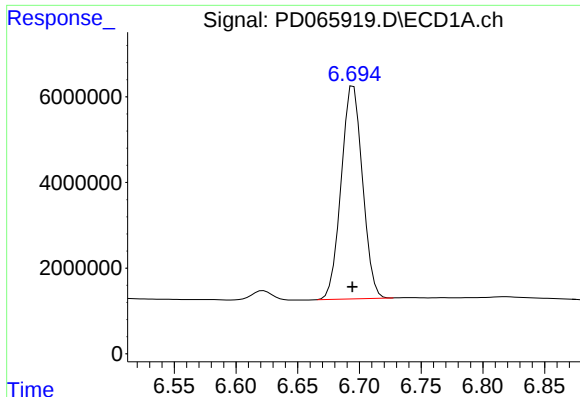

#19 Endosulfan Sulfate


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 59840281
Conc: 52.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

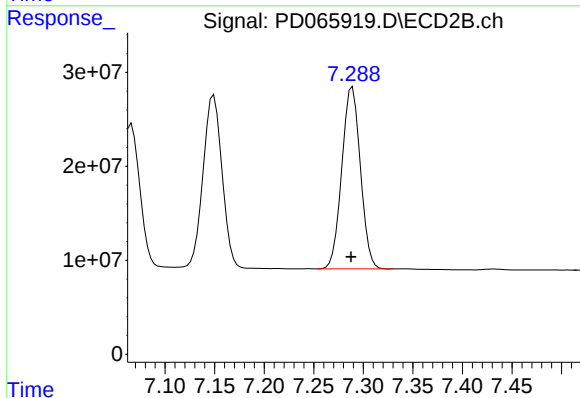


#19 Endosulfan Sulfate

R.T.: 7.289 min
Delta R.T.: 0.001 min
Response: 252508074
Conc: 51.19 ng/ml

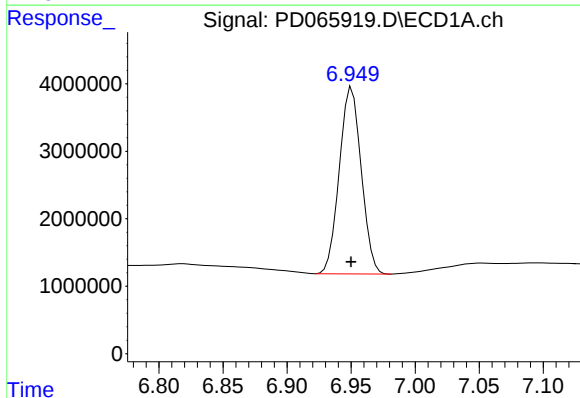


#20 Methoxychlor

R.T.: 6.951 min
Delta R.T.: 0.000 min
Response: 32934764
Conc: 48.20 ng/ml

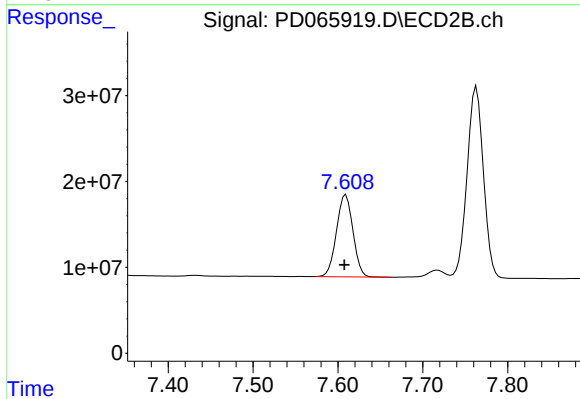

#20 Methoxychlor


R.T.: 7.609 min
Delta R.T.: 0.002 min
Response: 128788241
Conc: 48.94 ng/ml

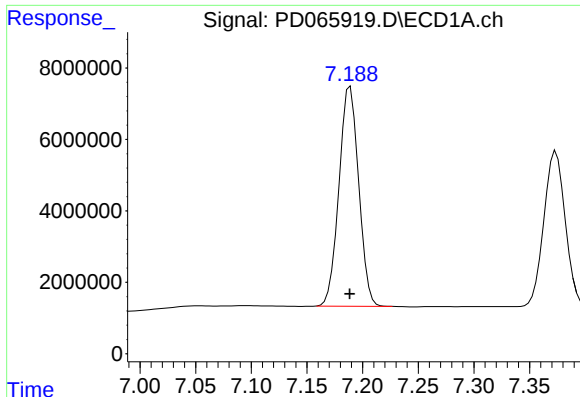

#21 Endrin ketone


R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 75763993
Conc: 53.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

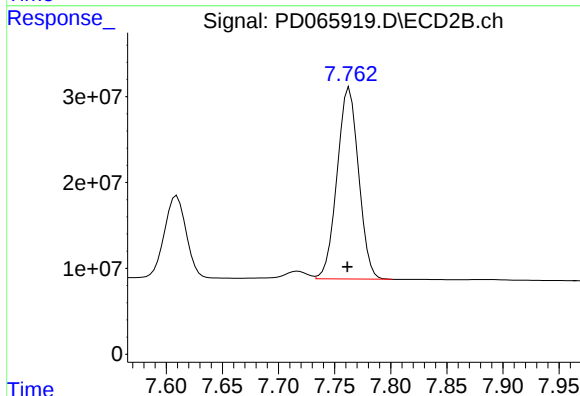


#21 Endrin ketone

R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 297319396
Conc: 52.13 ng/ml

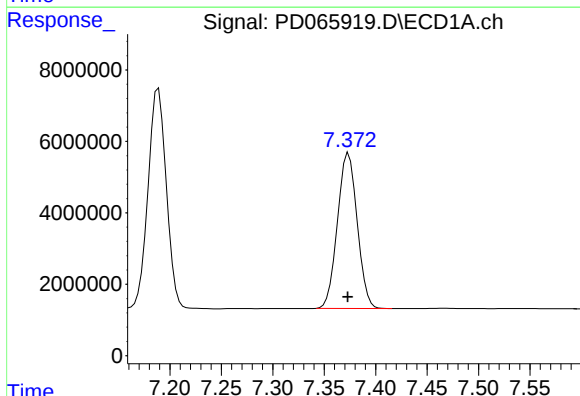


#22 Mirex

R.T.: 7.374 min
Delta R.T.: 0.000 min
Response: 58140028
Conc: 48.15 ng/ml

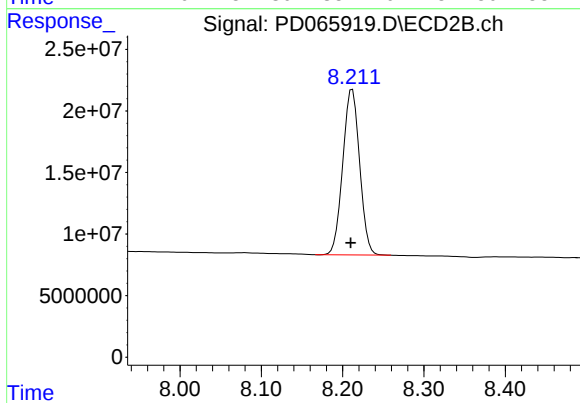

#22 Mirex


R.T.: 8.212 min
Delta R.T.: 0.002 min
Response: 193191495
Conc: 48.93 ng/ml

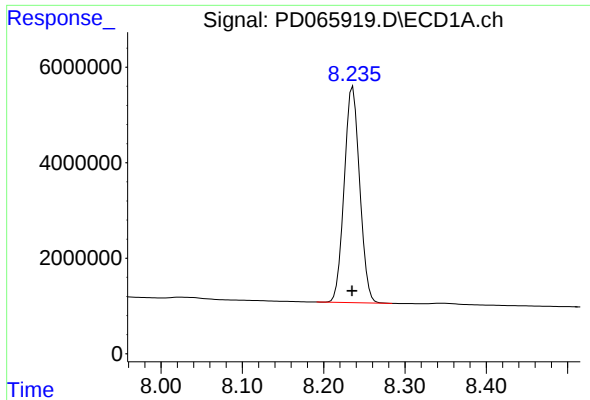

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.001 min
Response: 59612287
Conc: 43.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

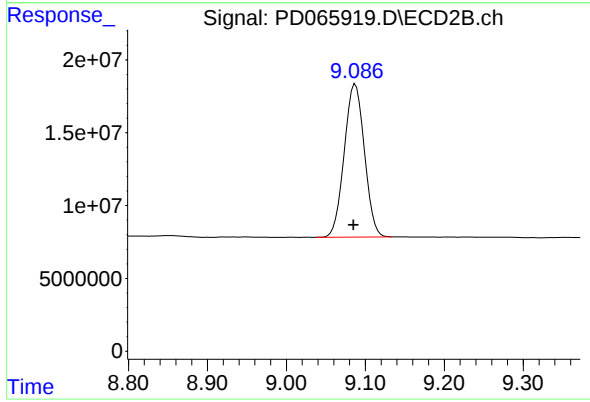

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.002 min
Response: 186532053
Conc: 48.20 ng/ml