

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
 Data File : PD065930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2021 00:15
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 02:15:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.013	38826706	289.9E6	52.429	50.488
28)	SA Decachlor...	8.235	9.086	55023280	178.0E6	40.282	45.981
Target Compounds							
2)	A alpha-BHC	3.933	4.408	60534652	424.5E6	53.901	50.487
3)	MA gamma-BHC...	4.216	4.694	59125624	389.4E6	52.726	50.407
4)	MA Heptachlor	4.513	5.197	62178886	349.9E6	52.128	48.219
5)	MB Aldrin	4.761	5.503	60409263	327.3E6	54.000	48.646
6)	B beta-BHC	4.464	4.870	29759520	177.2E6	52.130	47.935
7)	B delta-BHC	4.668	5.087	61245119	370.1E6	54.176	51.423
8)	B Heptachlo...	5.203	5.893	59681854	303.9E6	53.300	58.805
9)	A Endosulfan I	5.542	6.250	56976220	282.0E6	52.390	51.027
10)	B gamma-Chl...	5.428	6.126	61757615	300.2E6	51.143	50.056
11)	B alpha-Chl...	5.487	6.198	61193211	295.0E6	51.693	49.157
12)	B 4,4'-DDE	5.649	6.356	57478332	289.4E6	52.804	50.184
13)	MA Dieldrin	5.784	6.509	60586478	299.7E6	52.274	50.863
14)	MA Endrin	6.042	6.727	50407027	225.3E6	47.637	45.701
15)	B Endosulfa...	6.315	6.941	53905355	242.7E6	49.898	50.096
16)	A 4,4'-DDD	6.164	6.851	51493358	246.3E6	52.494	50.113
17)	MA 4,4'-DDT	6.404	7.148	52971866	239.8E6	48.126	47.463
18)	B Endrin al...	6.483	7.066	43660814	193.9E6	49.264	49.518
19)	B Endosulfa...	6.695	7.288	58030418	243.2E6	50.843	49.307
20)	A Methoxychlor	6.951	7.608	32191803	124.1E6	47.108	47.148
21)	B Endrin ke...	7.189	7.762	70950502	280.7E6	50.368	49.217
22)	Mirex	7.374	8.210	54940045	182.3E6	45.504	46.162



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
Data File : PD065930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2021 00:15
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 02:15:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

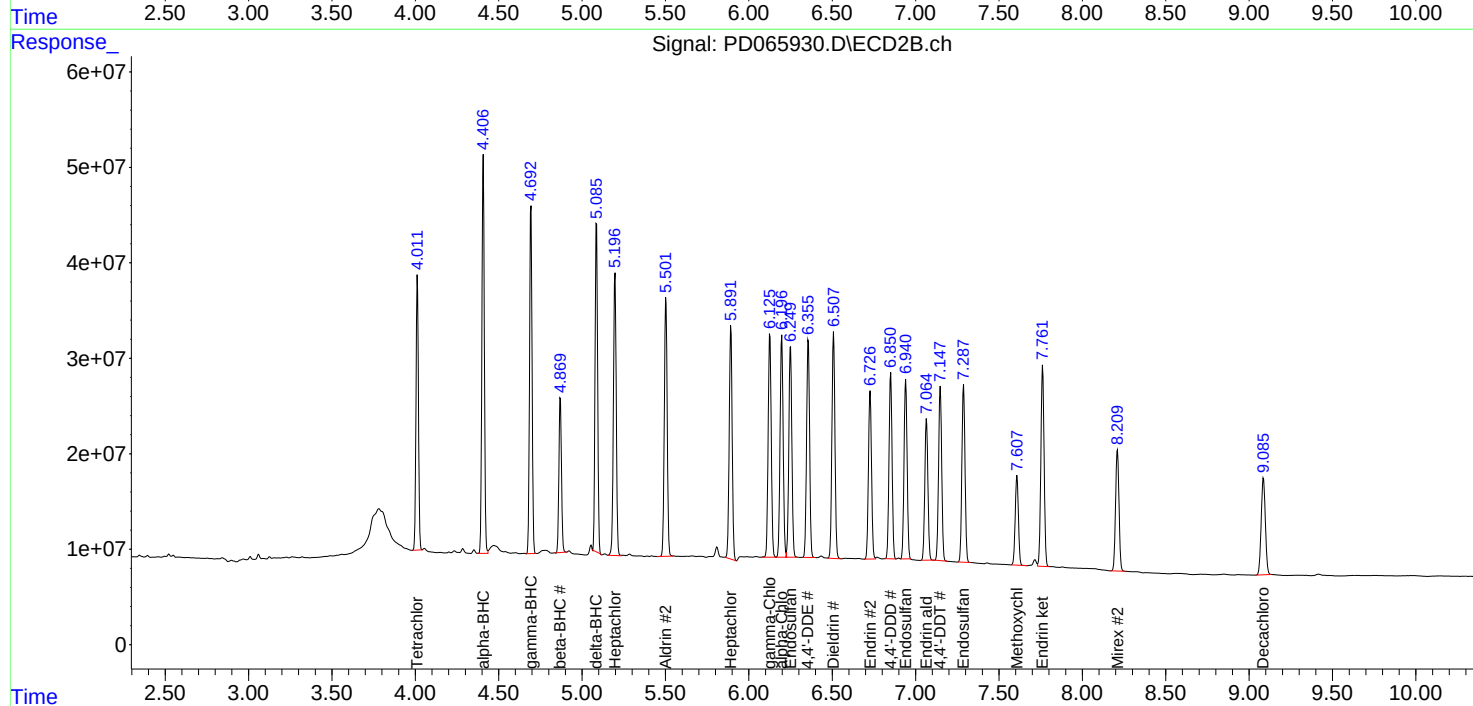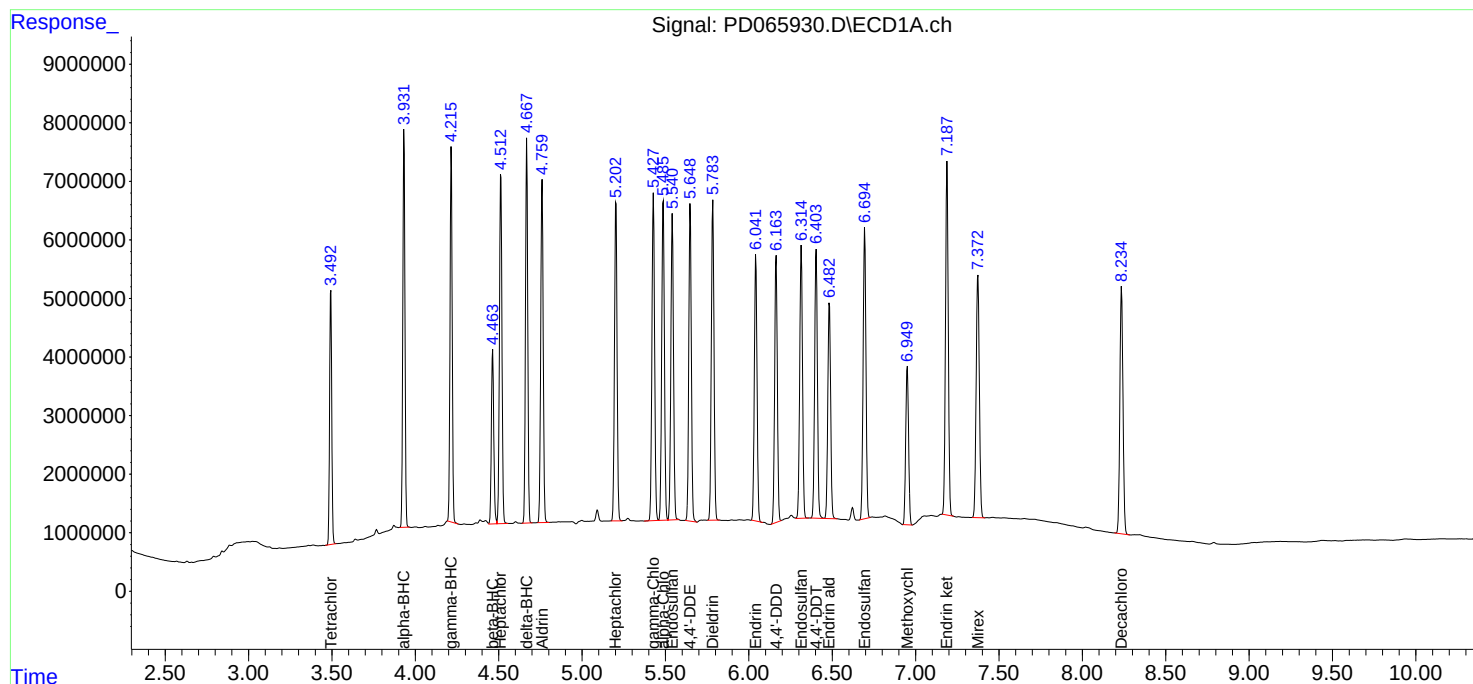


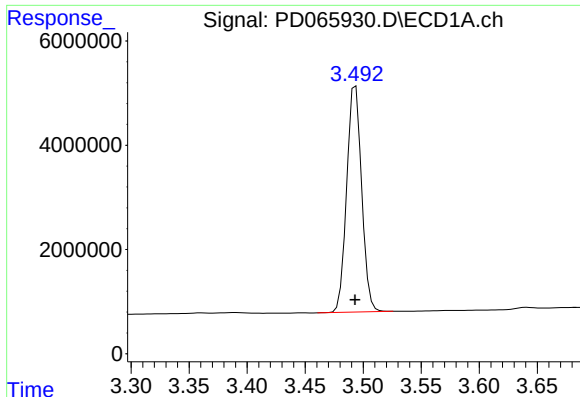

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 38826706
Conc: 52.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

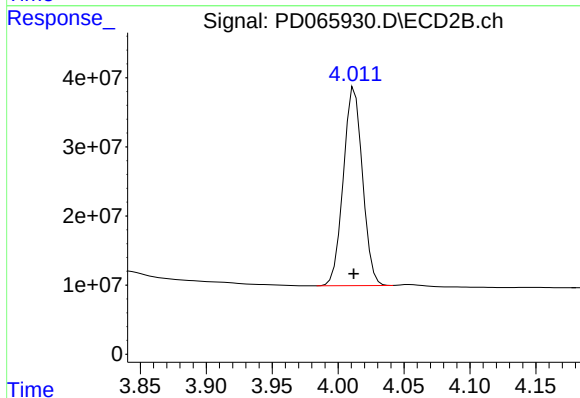


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 289907169
Conc: 50.49 ng/ml

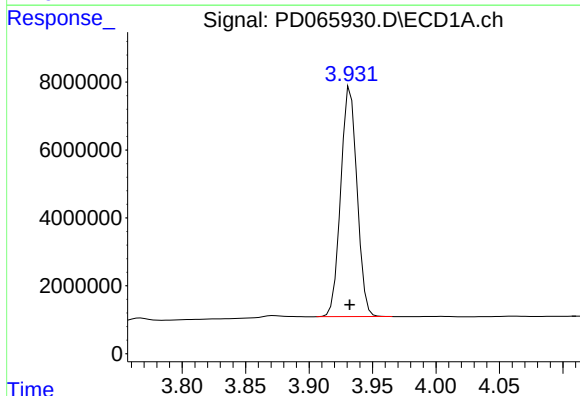


#2 alpha-BHC

R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 60534652
Conc: 53.90 ng/ml

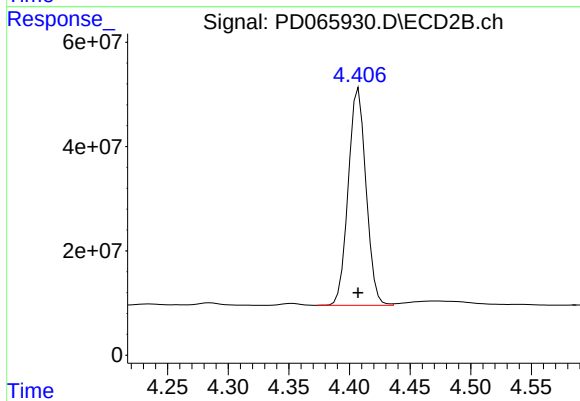

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 424502265
Conc: 50.49 ng/ml

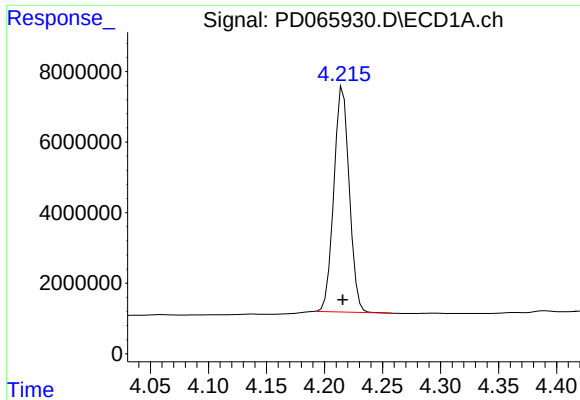

#3 gamma-BHC (Lindane)


R.T.: 4.216 min
Delta R.T.: 0.000 min
Response: 59125624
Conc: 52.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

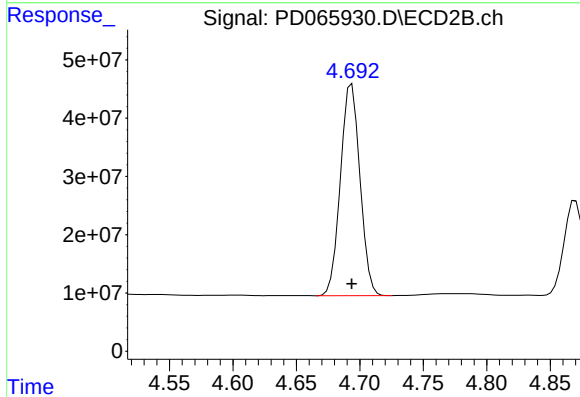


#3 gamma-BHC (Lindane)

R.T.: 4.694 min
Delta R.T.: 0.000 min
Response: 389436455
Conc: 50.41 ng/ml

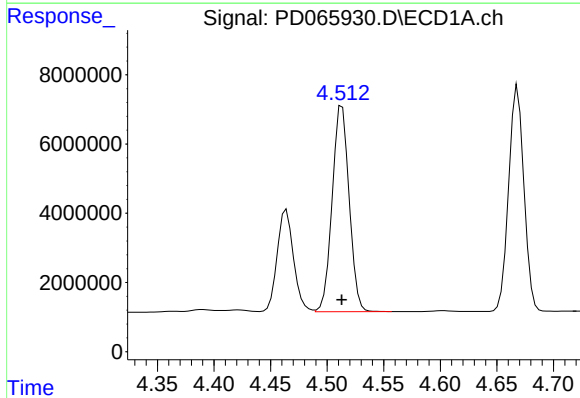


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 62178886
Conc: 52.13 ng/ml

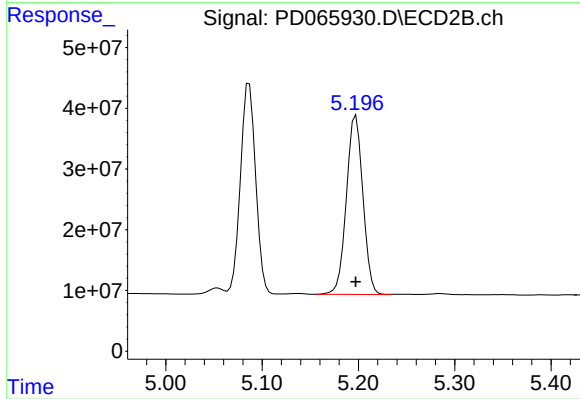

#4 Heptachlor


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 349862684
Conc: 48.22 ng/ml

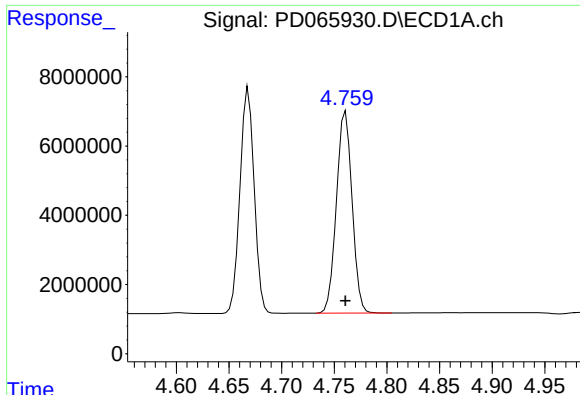

#5 Aldrin


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 60409263
Conc: 54.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

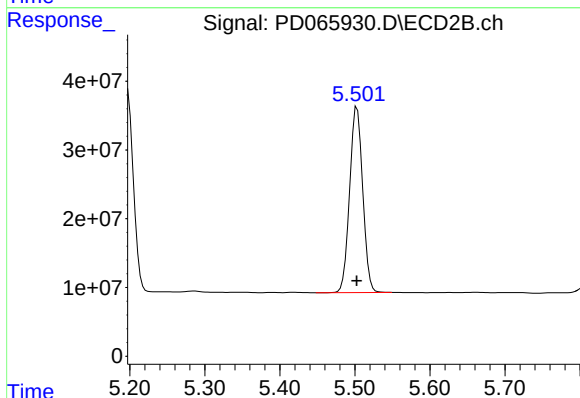


#5 Aldrin

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 327272703
Conc: 48.65 ng/ml

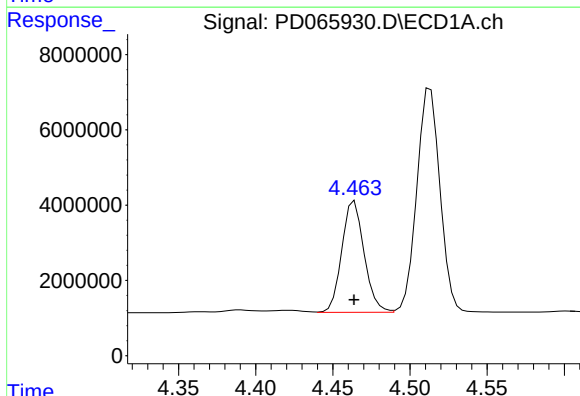


#6 beta-BHC

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 29759520
Conc: 52.13 ng/ml

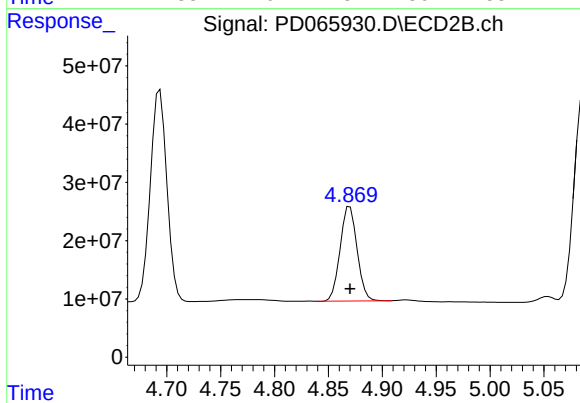

#6 beta-BHC


R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 177158836
Conc: 47.93 ng/ml

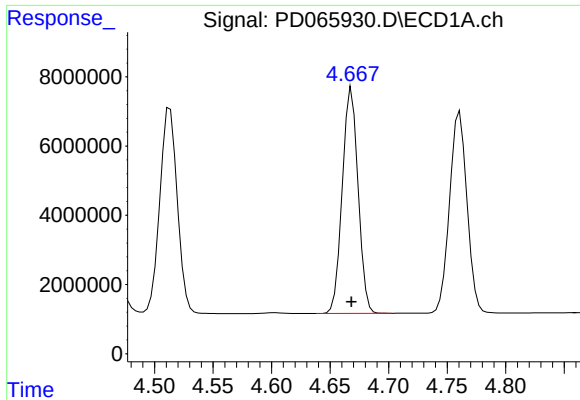

#7 delta-BHC


R.T.: 4.668 min
Delta R.T.: 0.000 min
Response: 61245119
Conc: 54.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

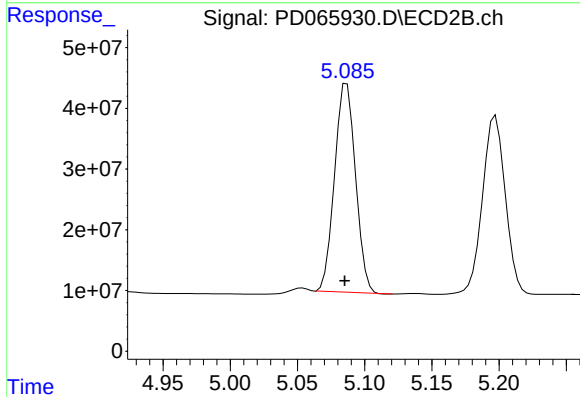


#7 delta-BHC

R.T.: 5.087 min
Delta R.T.: 0.002 min
Response: 370078199
Conc: 51.42 ng/ml

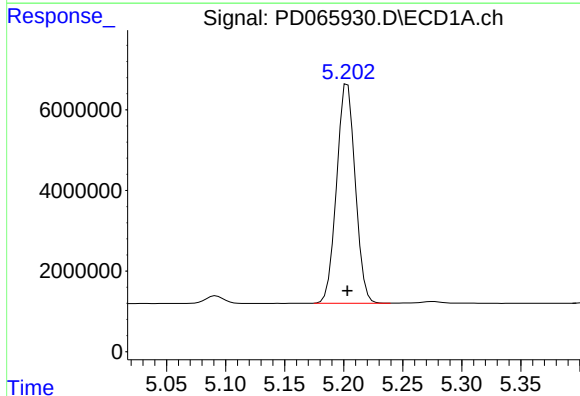


#8 Heptachlor epoxide

R.T.: 5.203 min
Delta R.T.: 0.000 min
Response: 59681854
Conc: 53.30 ng/ml

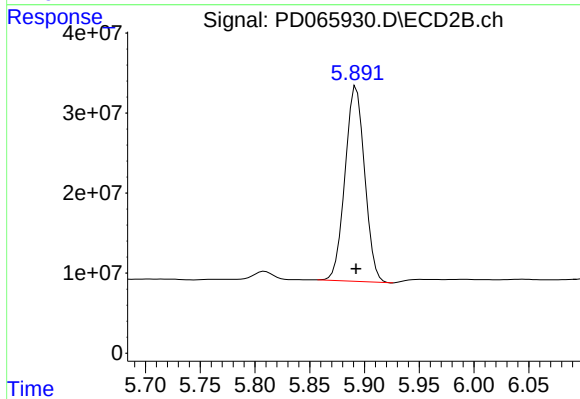

#8 Heptachlor epoxide


R.T.: 5.893 min
Delta R.T.: 0.000 min
Response: 303897635
Conc: 58.81 ng/ml

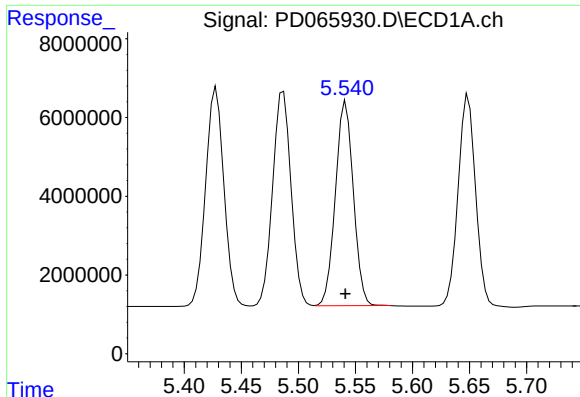

#9 Endosulfan I


R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 56976220
Conc: 52.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

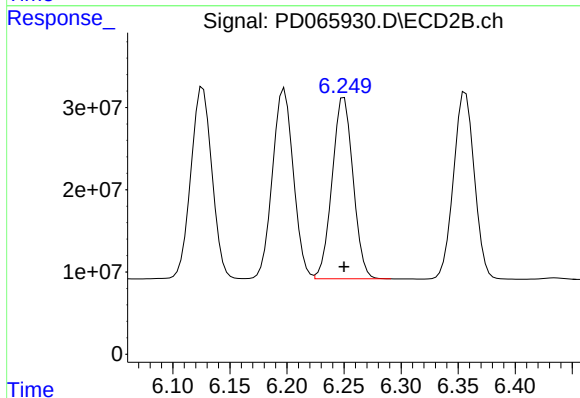


#9 Endosulfan I

R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 282027658
Conc: 51.03 ng/ml

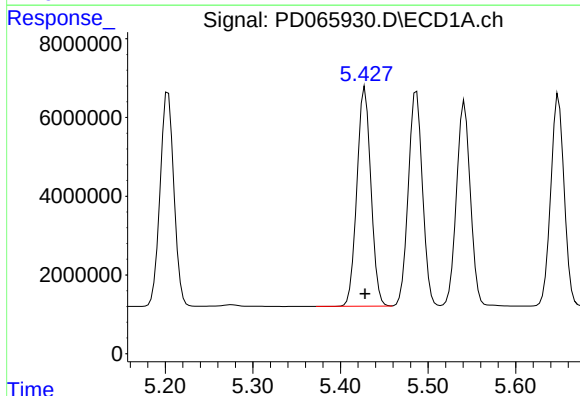


#10 gamma-Chlordane

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 61757615
Conc: 51.14 ng/ml

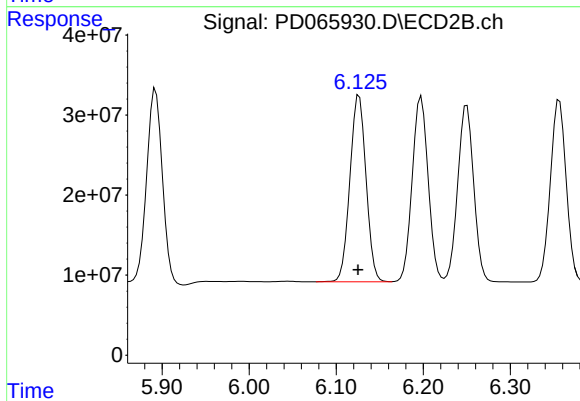

#10 gamma-Chlordane


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 300224631
Conc: 50.06 ng/ml

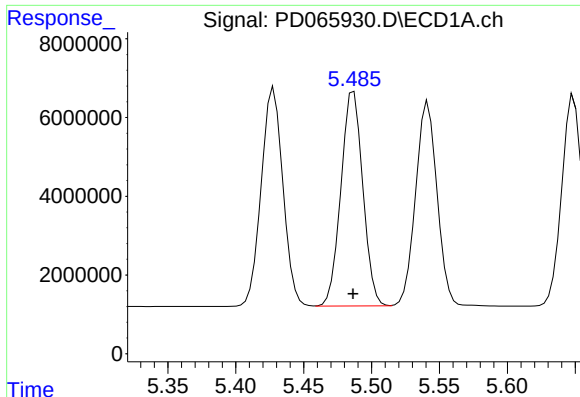

#11 alpha-Chlordane


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 61193211
Conc: 51.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

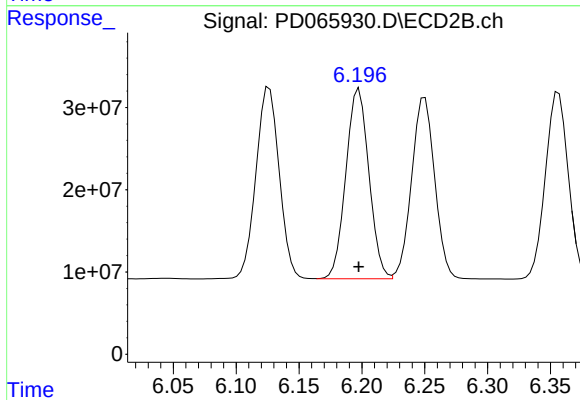


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 295040325
Conc: 49.16 ng/ml

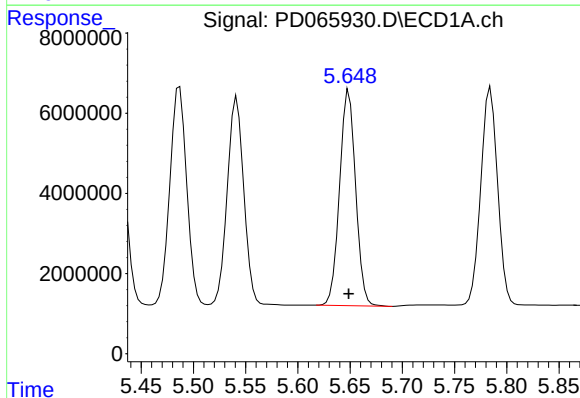


#12 4,4'-DDE

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 57478332
Conc: 52.80 ng/ml

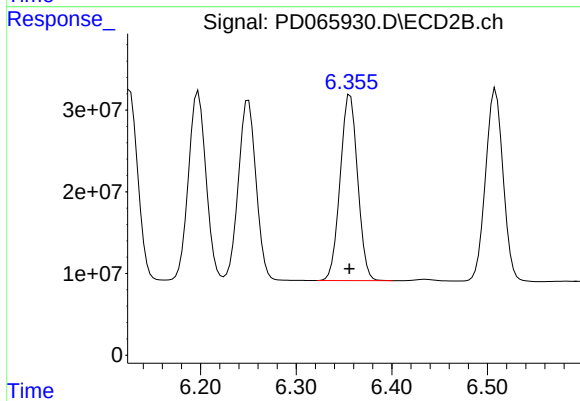

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 289436484
Conc: 50.18 ng/ml

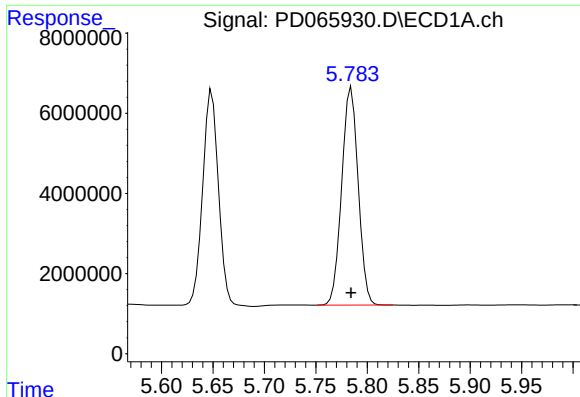

#13 Dieldrin


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 60586478
Conc: 52.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

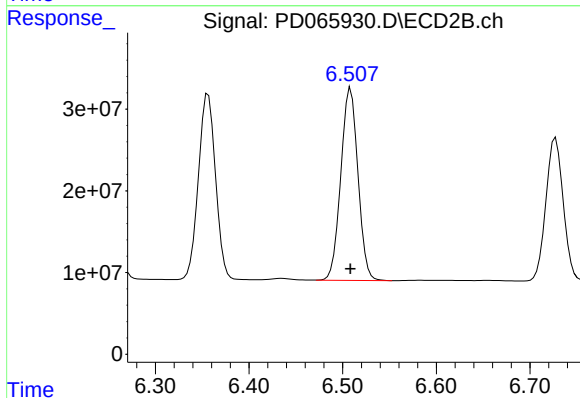


#13 Dieldrin

R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 299744553
Conc: 50.86 ng/ml

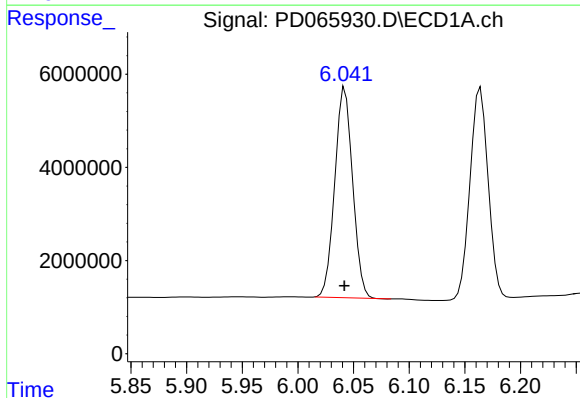


#14 Endrin

R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 50407027
Conc: 47.64 ng/ml

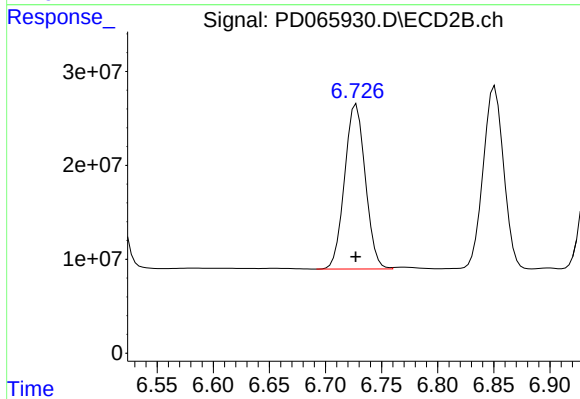

#14 Endrin


R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 225311124
Conc: 45.70 ng/ml

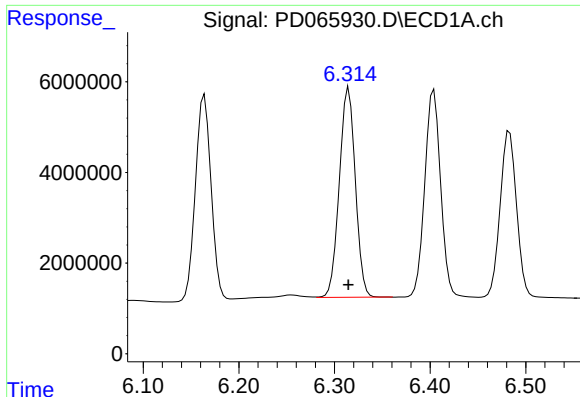

#15 Endosulfan II


R.T.: 6.315 min
Delta R.T.: 0.000 min
Response: 53905355
Conc: 49.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

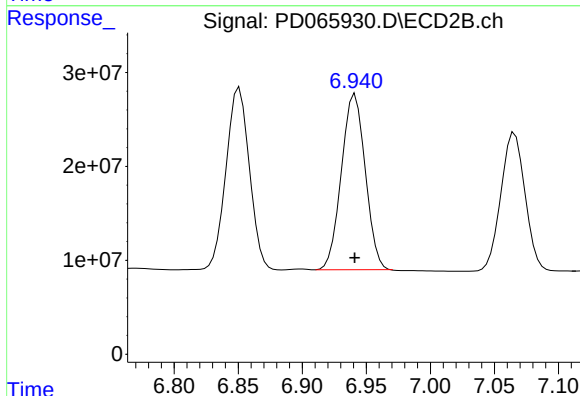


#15 Endosulfan II

R.T.: 6.941 min
Delta R.T.: 0.000 min
Response: 242660432
Conc: 50.10 ng/ml

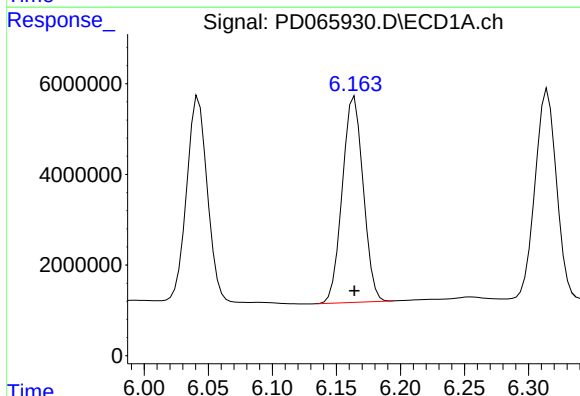


#16 4,4'-DDD

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 51493358
Conc: 52.49 ng/ml

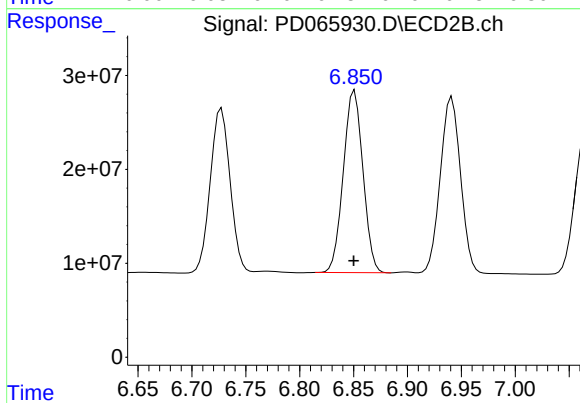

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 246285501
Conc: 50.11 ng/ml

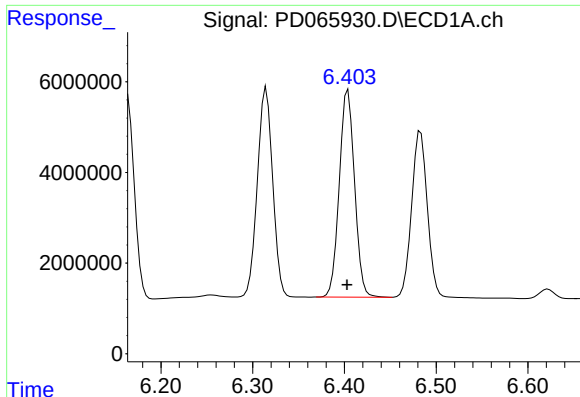

#17 4,4'-DDT


R.T.: 6.404 min
Delta R.T.: 0.001 min
Response: 52971866
Conc: 48.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

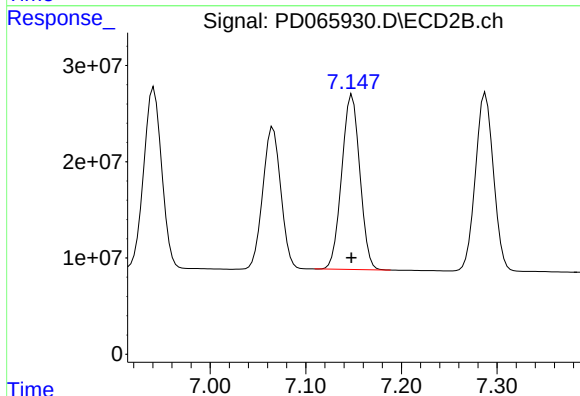


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 239753564
Conc: 47.46 ng/ml

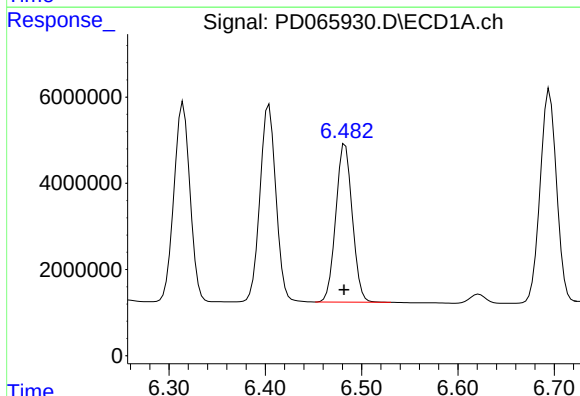


#18 Endrin aldehyde

R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 43660814
Conc: 49.26 ng/ml

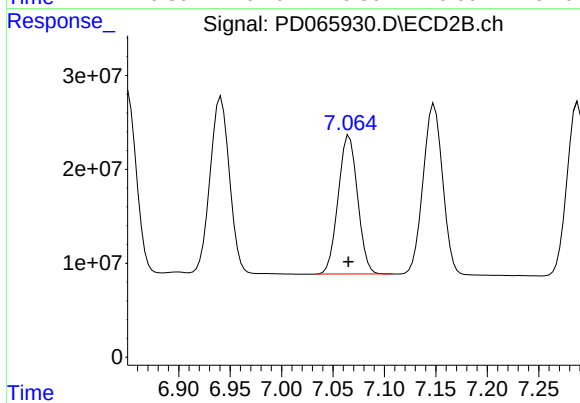

#18 Endrin aldehyde


R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 193858946
Conc: 49.52 ng/ml

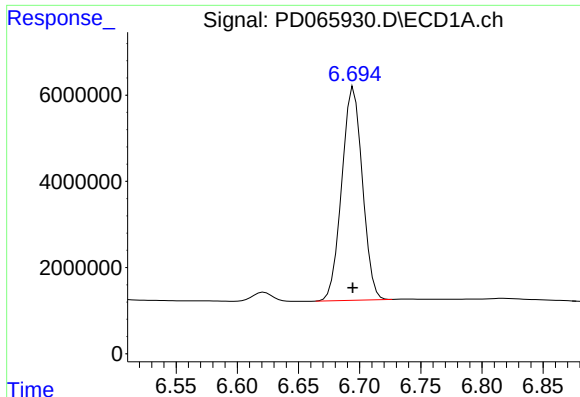

#19 Endosulfan Sulfate


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 58030418
Conc: 50.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

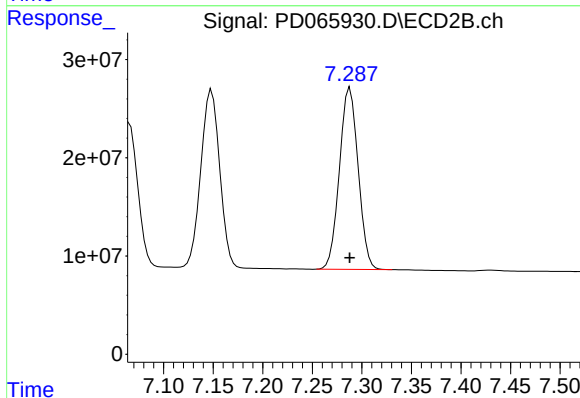


#19 Endosulfan Sulfate

R.T.: 7.288 min
Delta R.T.: 0.000 min
Response: 243197598
Conc: 49.31 ng/ml

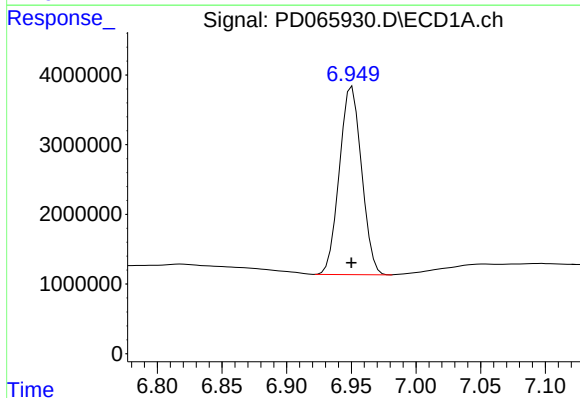


#20 Methoxychlor

R.T.: 6.951 min
Delta R.T.: 0.000 min
Response: 32191803
Conc: 47.11 ng/ml

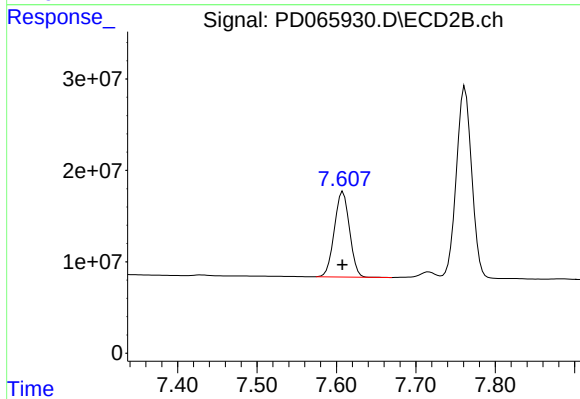

#20 Methoxychlor


R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 124074340
Conc: 47.15 ng/ml

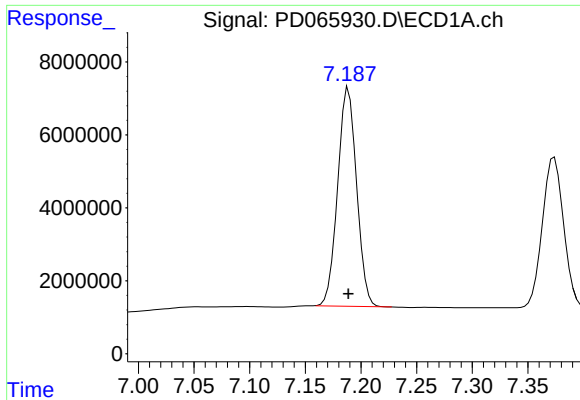

#21 Endrin ketone


R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 70950502
Conc: 50.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

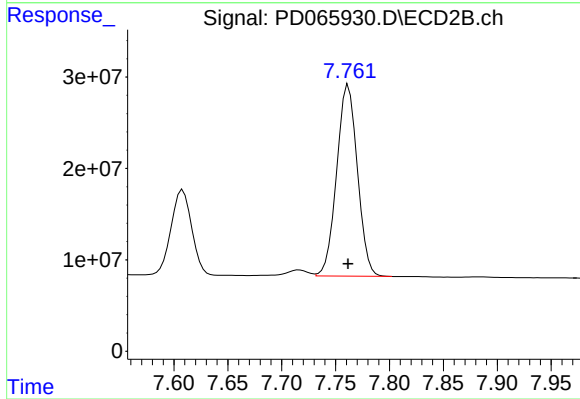


#21 Endrin ketone

R.T.: 7.762 min
Delta R.T.: 0.000 min
Response: 280682426
Conc: 49.22 ng/ml

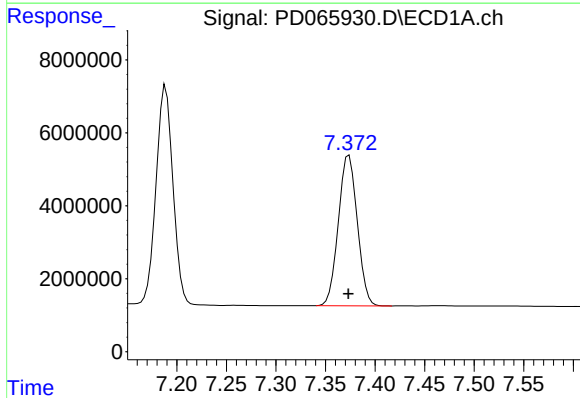


#22 Mirex

R.T.: 7.374 min
Delta R.T.: 0.000 min
Response: 54940045
Conc: 45.50 ng/ml

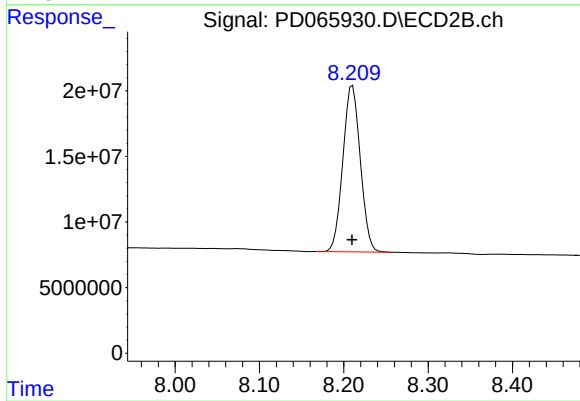

#22 Mirex


R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 182276108
Conc: 46.16 ng/ml

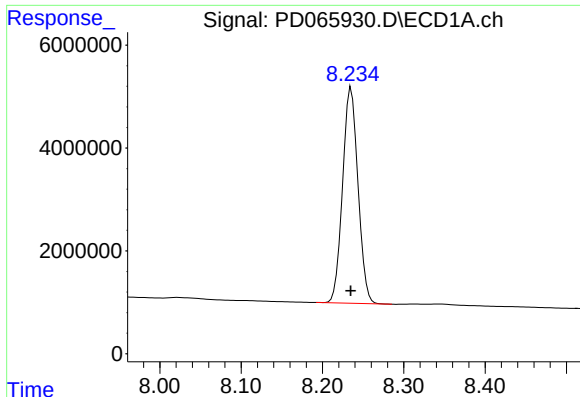

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 55023280
Conc: 40.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

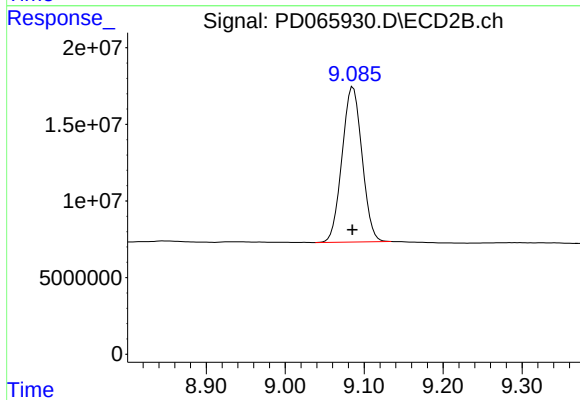

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 177952107
Conc: 45.98 ng/ml