

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
 Data File : PD065931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2021 01:24
 Operator : AR\AJ
 Sample : M3946-01 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PL-05-092421

Manual Integrations
 APPROVED

mohammad
 9/28/2021 11:28:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 02:23:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.493	4.013	2858245	22046874	3.860	3.839
28) SA Decachlor...	8.235	9.084	4493475	19300502	3.290	4.987m#
Target Compounds						
16) A 4,4'-DDD	6.167	6.851	500048	6831368	0.510m	1.390 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092721\
Data File : PD065931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2021 01:24
Operator : AR\AJ
Sample : M3946-01 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PL-05-092421


Manual Integrations
APPROVED

mohammad
9/28/2021 11:28:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 02:23:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

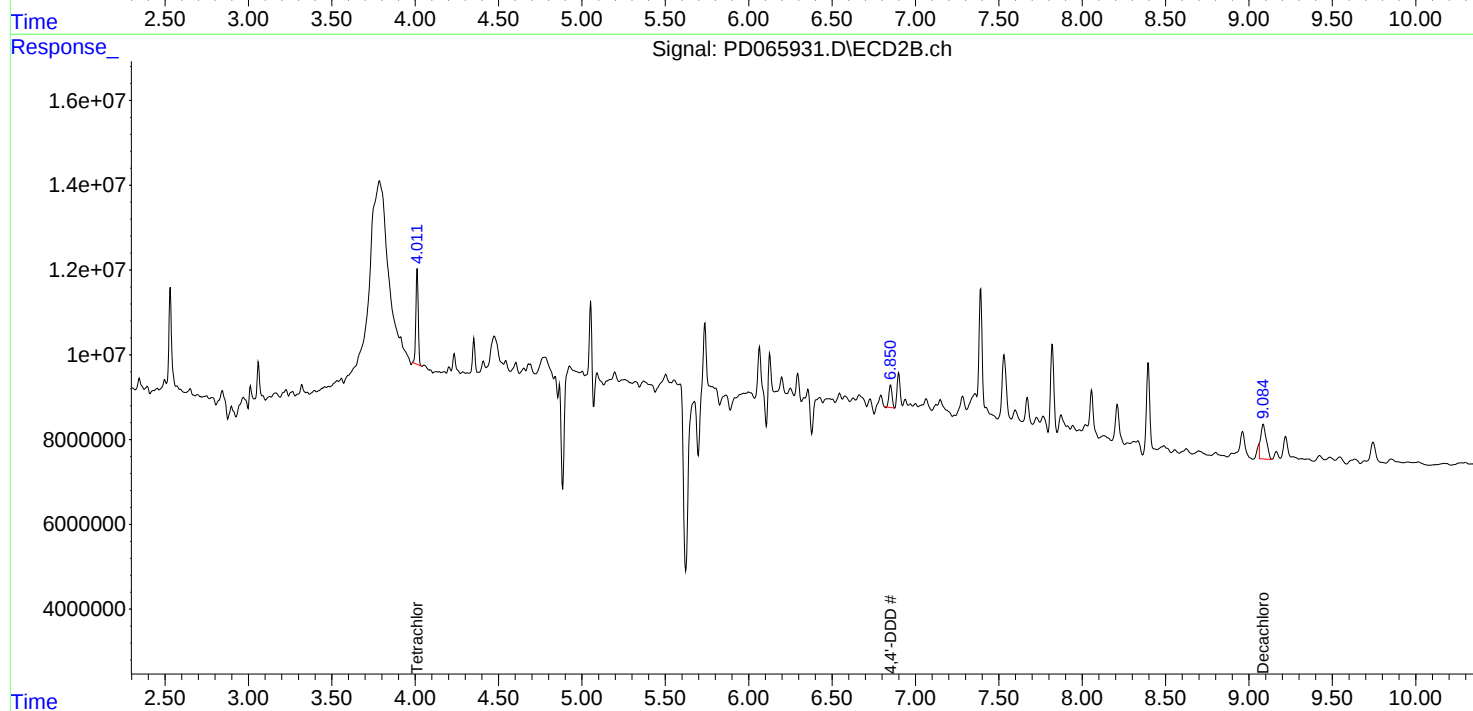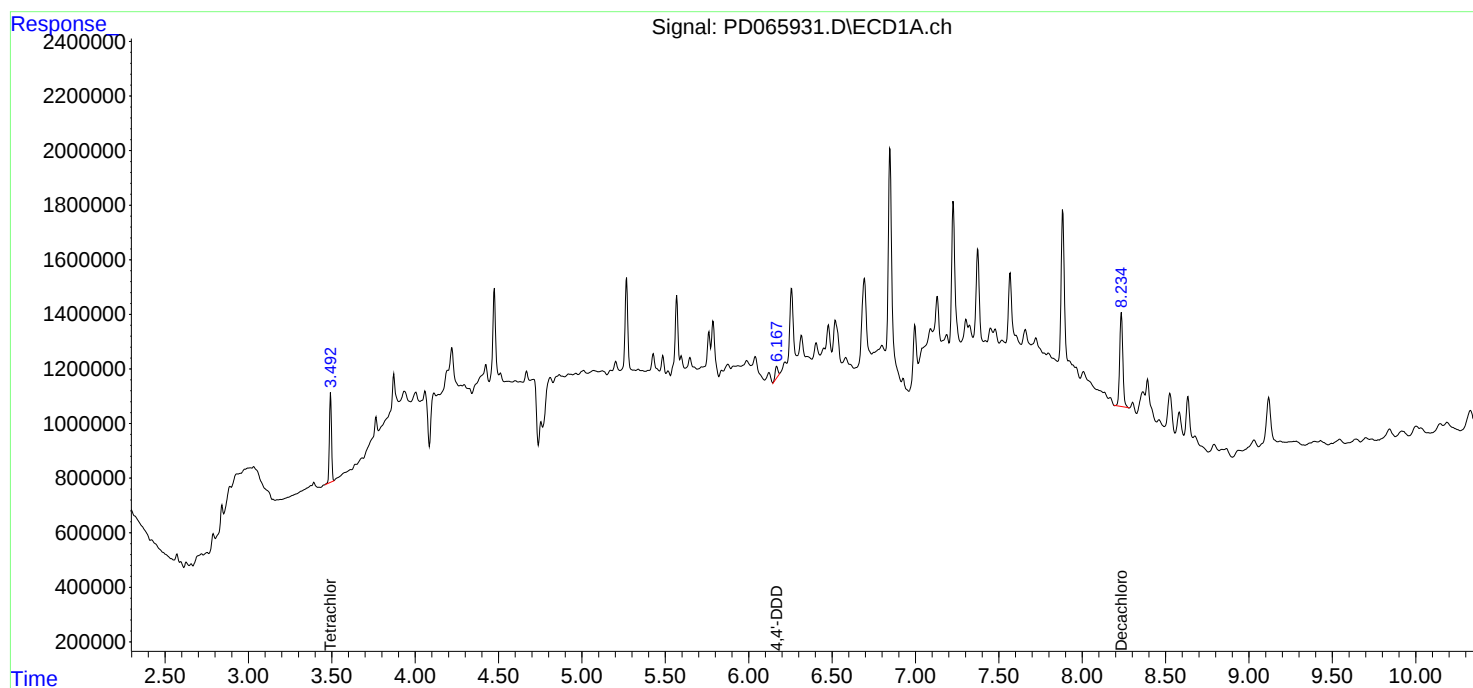

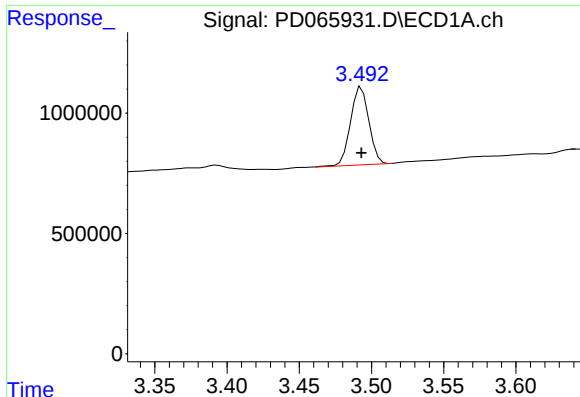


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 2858245
Conc: 3.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PL-05-092421


Manual Integrations
APPROVED

mohammad
9/28/2021 11:28:13 AM

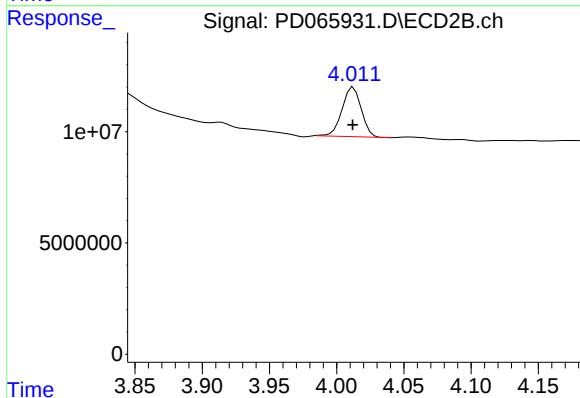


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 22046874
Conc: 3.84 ng/ml

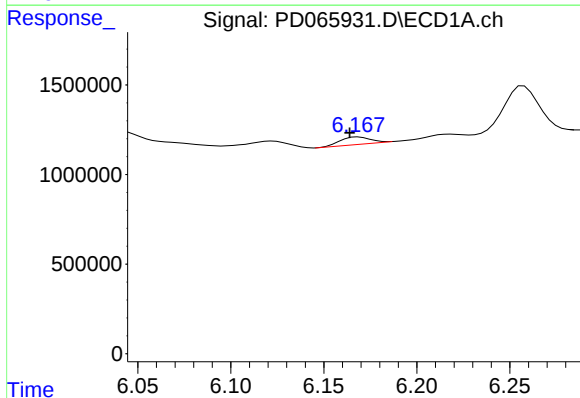


#16 4,4'-DDD

R.T.: 6.167 min
Delta R.T.: 0.003 min
Response: 500048
Conc: 0.51 ng/ml m

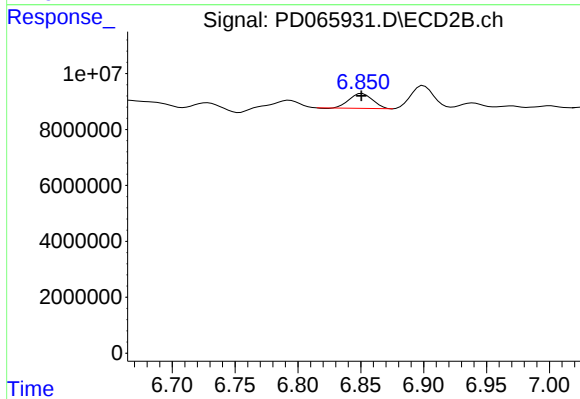

#16 4,4'-DDD

R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 6831368
Conc: 1.39 ng/ml

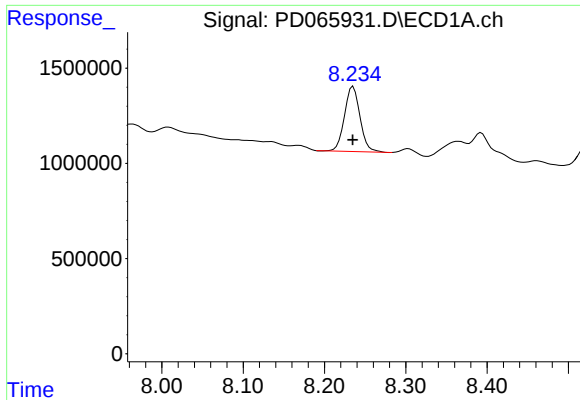


#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 4493475
Conc: 3.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PL-05-092421

Manual Integrations
APPROVED

mohammad
9/28/2021 11:28:13 AM

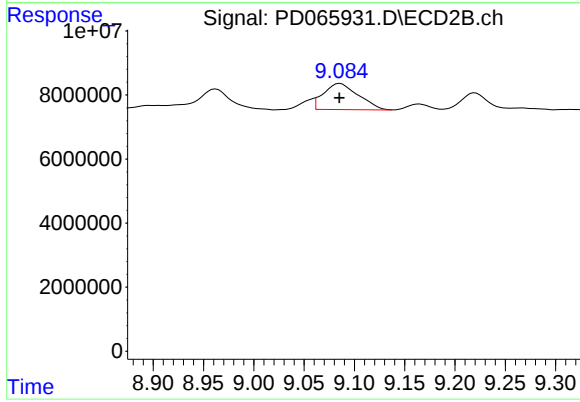

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 19300502
Conc: 4.99 ng/ml m