

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092722\
 Data File : PS020655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2022 08:51
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:39:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.750	1524023	2203769	<MDL	2.588 #
Target Compounds							
1) T	Dalapon	3.050f	0.000	752027	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.441f	0.000	5233923	0	1.050	N.D. #
3) T	4-Nitroph...	7.060	0.000	6317465	0	130.387	N.D. #
5) T	DICAMBA	7.405f	0.000	1592433	0	<MDL	N.D. #
6) T	MCP	7.531	7.001	3428768	529744	<MDL	<MDL #
7) T	MCPA	7.679	0.000	5033420	0	<MDL	N.D. #
9) T	2,4-D	8.279	0.000	80163129	0	17.247	N.D. #
10) T	Pentachlo...	8.600	0.000	1631699	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.110	0.000	511266	0	<MDL	N.D. #
12) T	2,4,5-T	9.395	0.000	7545193	0	<MDL	N.D. #
15) T	Picloram	10.954	10.848	28912740	3553688	<MDL	<MDL #
16) T	DCPA	11.371	0.000	7136539	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092722\
Data File : PS020655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2022 08:51
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:39:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

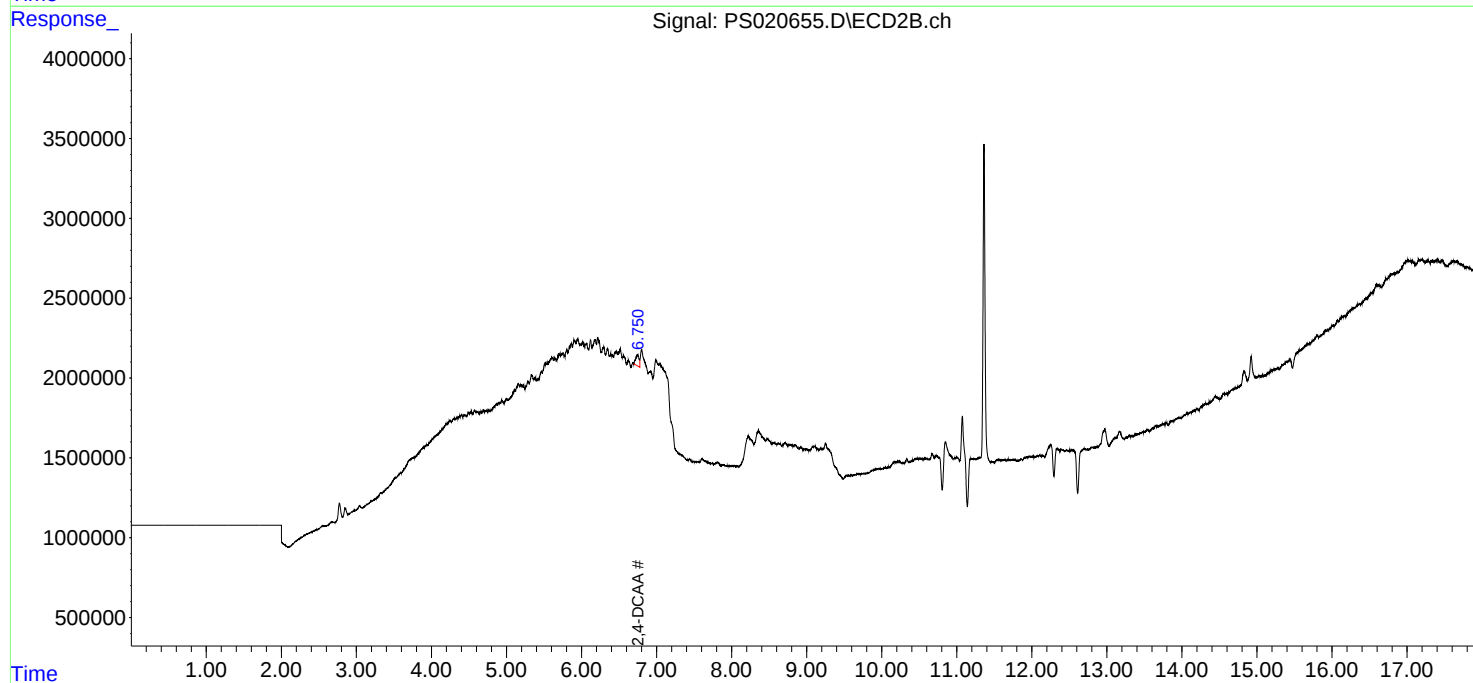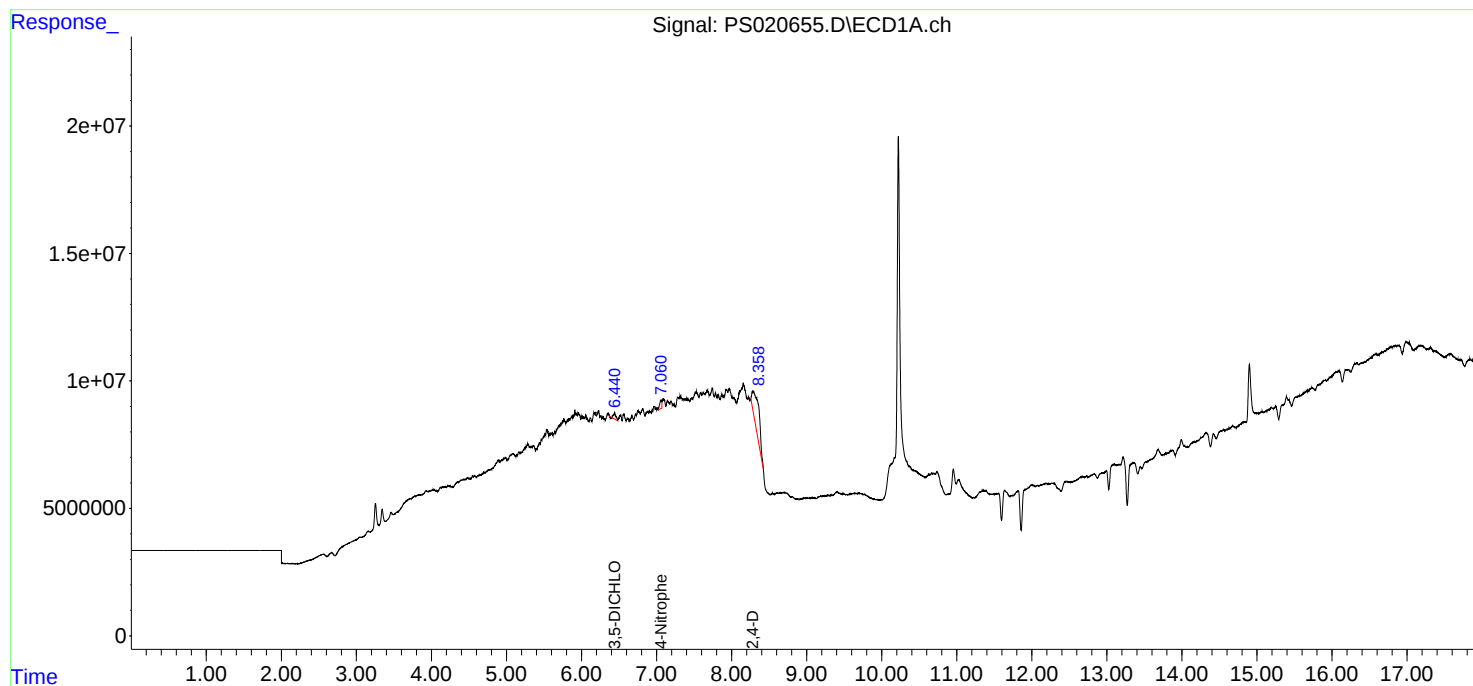


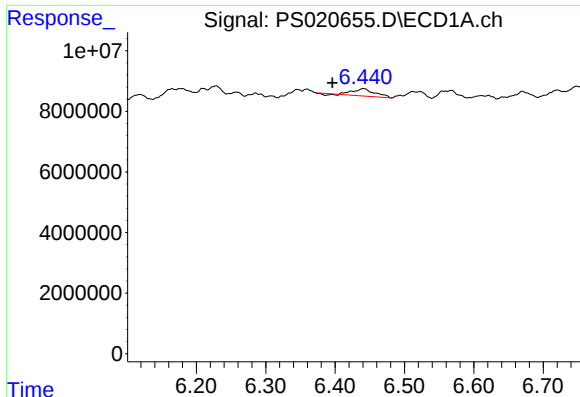

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.441 min
Delta R.T.: 0.045 min
Response: 5233923
Conc: 1.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

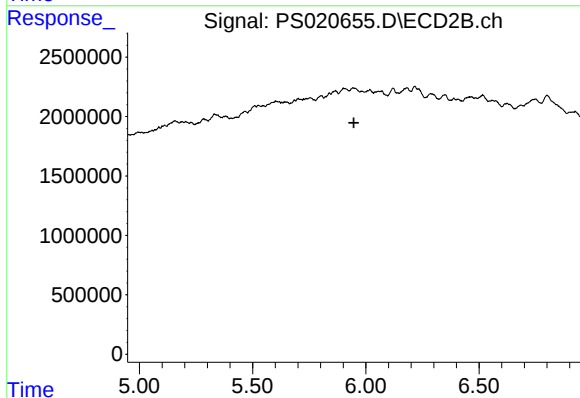


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

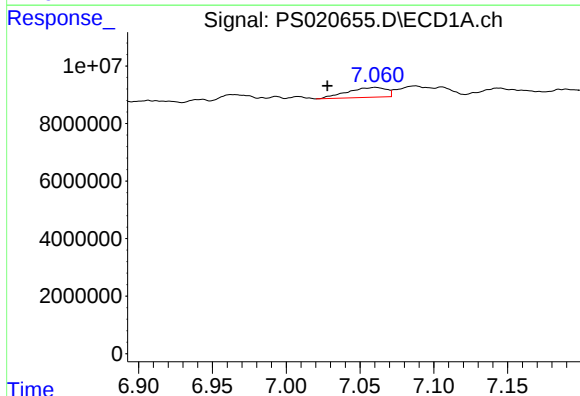


#3 4-Nitrophenol

R.T.: 7.060 min
Delta R.T.: 0.032 min
Response: 6317465
Conc: 130.39 ng/ml

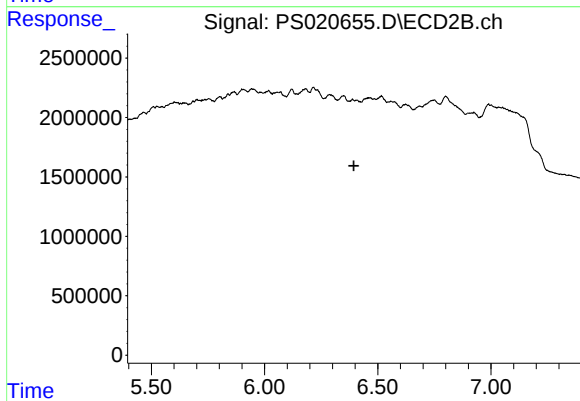

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

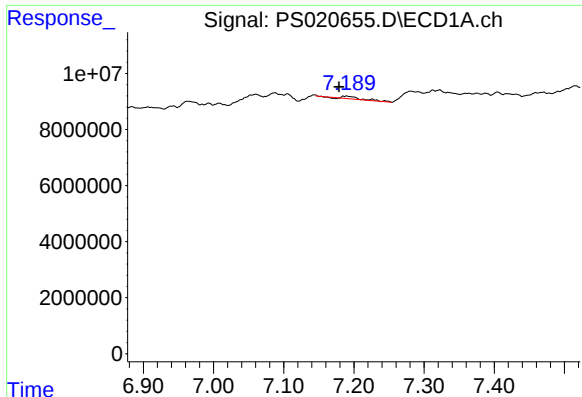

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: 0.010 min
Response: 1524023
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

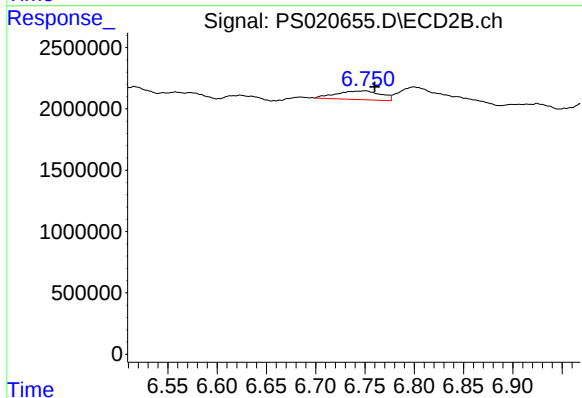


#4 2,4-DCAA

R.T.: 6.750 min
Delta R.T.: -0.010 min
Response: 2203769
Conc: 2.59 ng/ml

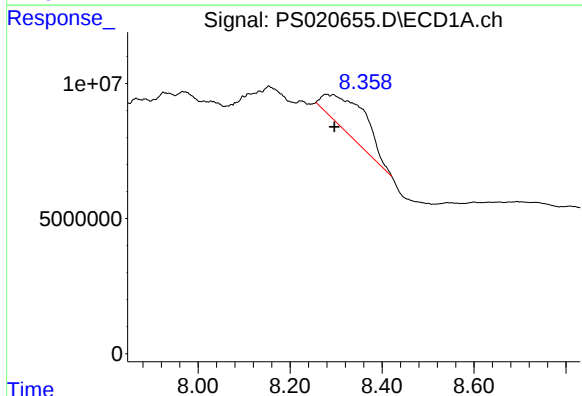

#9 2,4-D

R.T.: 8.279 min
Delta R.T.: -0.018 min
Response: 80163129
Conc: 17.25 ng/ml

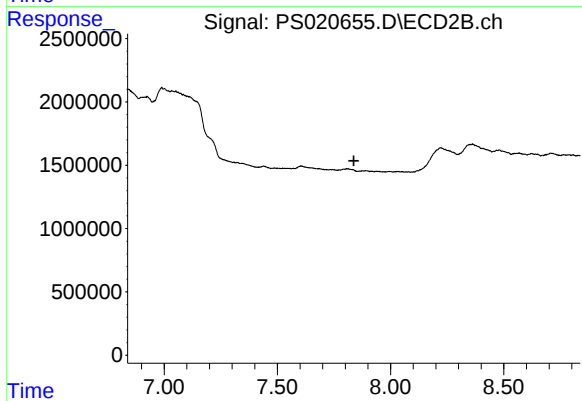

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.