

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092722\
 Data File : PS020656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2022 09:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:40:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.762	1612.3E6	447.6E6	468.477	525.567
Target Compounds							
1) T	Dalapon	2.986	0.000	180575	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.461f	0.000	2198490	0	<MDL	N.D. #
3) T	4-Nitroph...	6.994	0.000	1055438	0	127.651	N.D. #
7) T	MCPA	7.646	0.000	867951	0	<MDL	N.D. #
9) T	2,4-D	8.358f	0.000	82182710	0	17.681	N.D. #
10) T	Pentachlo...	8.538f	0.000	795717	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.078f	0.000	1916031	0	<MDL	N.D. #
13) T	2,4-DB	10.035f	0.000	174302	0	<MDL	N.D. #
14) T	DINOSEB	11.135	0.000	32163139	0	1.751	N.D. #
15) T	Picloram	10.920f	0.000	475917	0	<MDL	N.D. #
16) T	DCPA	11.404	0.000	2249689	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092722\
Data File : PS020656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2022 09:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:40:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

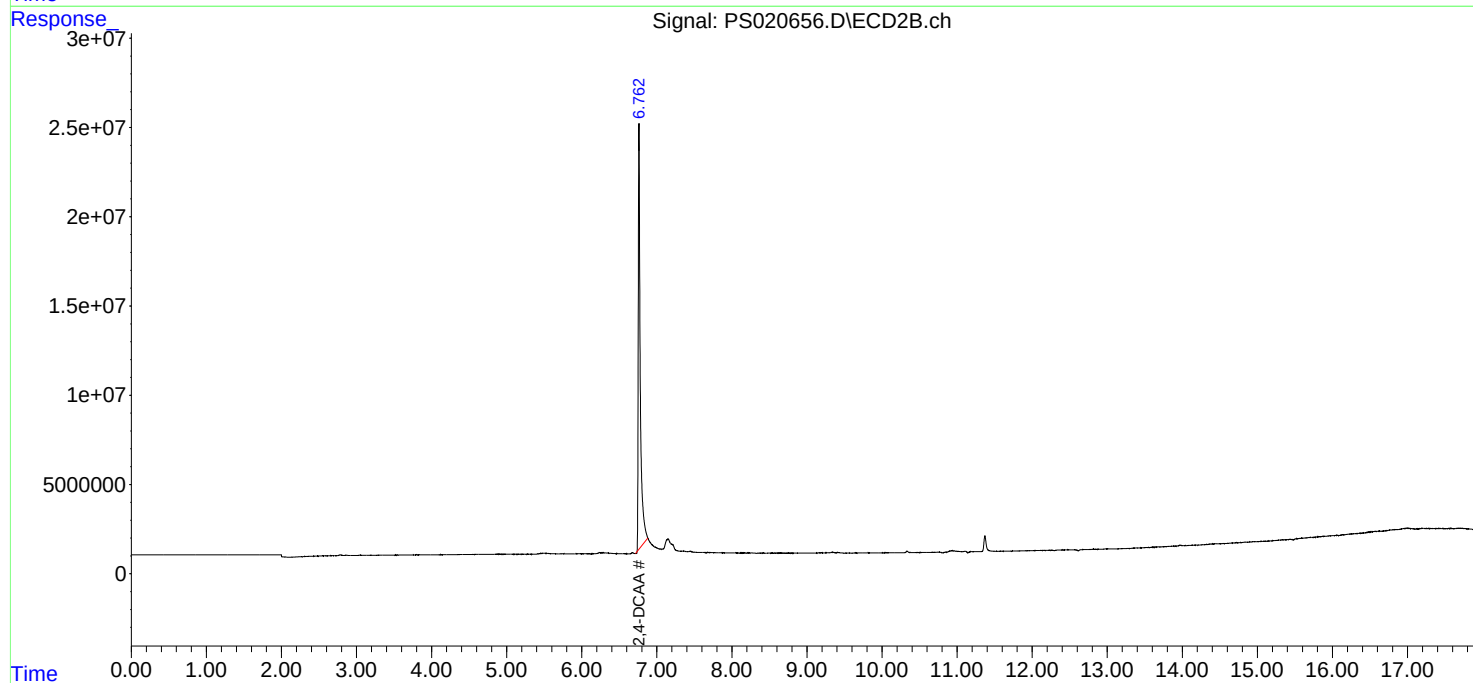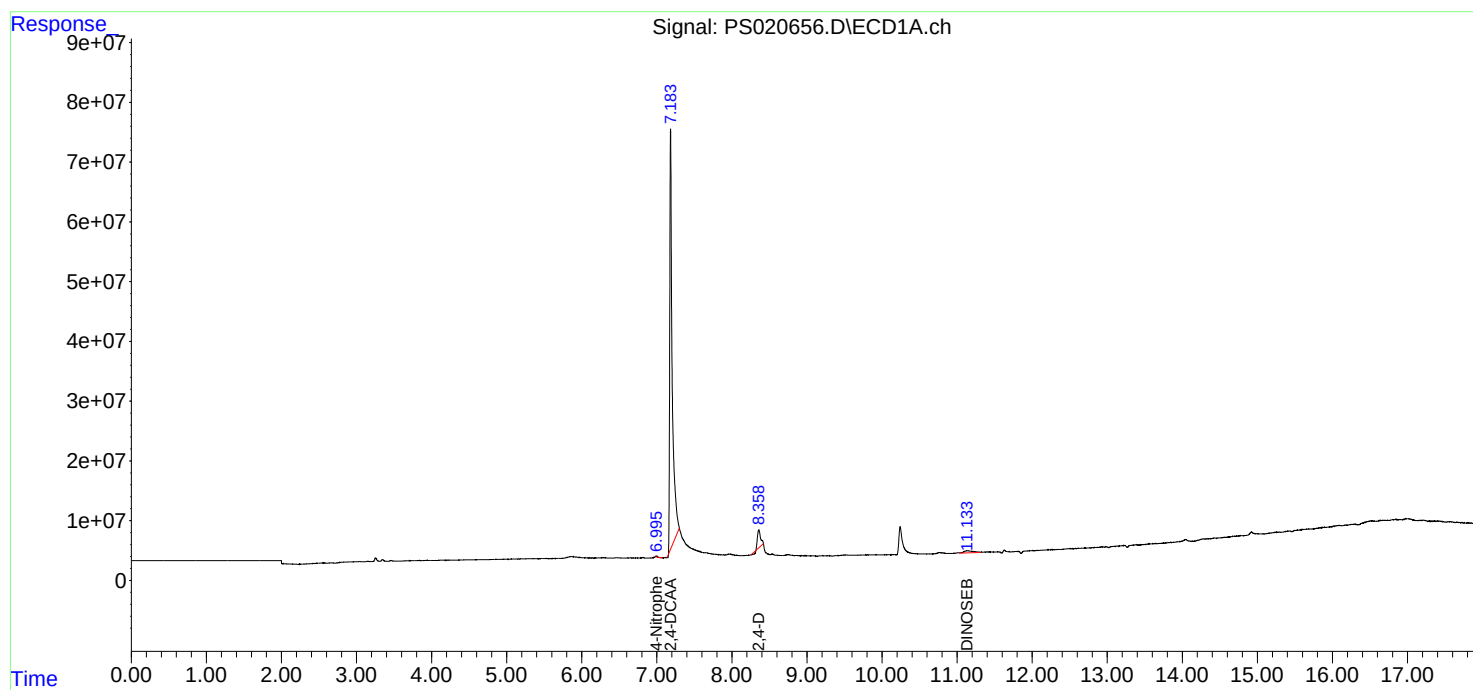


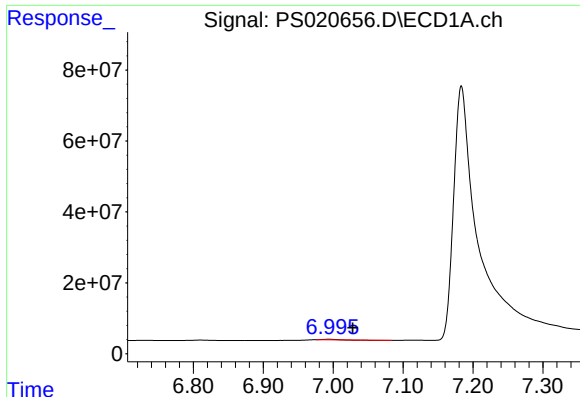

#3 4-Nitrophenol


R.T.: 6.994 min
Delta R.T.: -0.034 min
Response: 1055438
Conc: 127.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

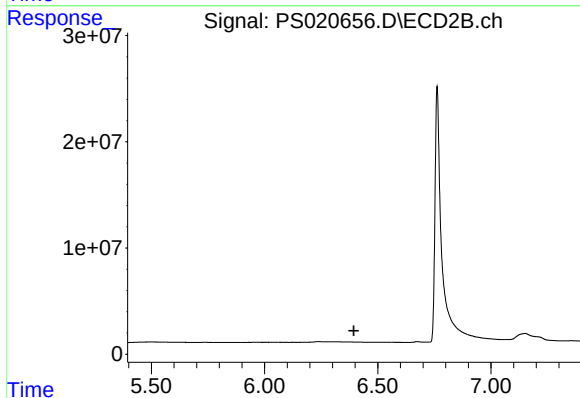


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

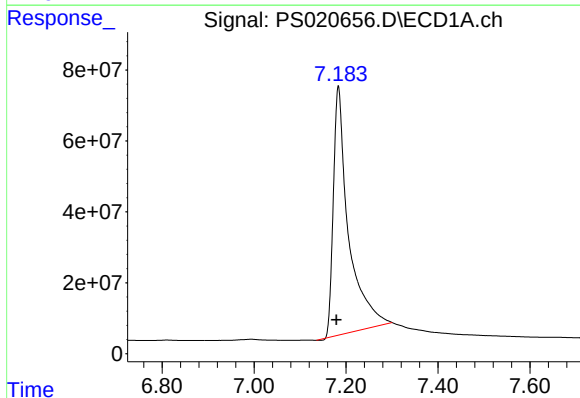


#4 2,4-DCAA

R.T.: 7.184 min
Delta R.T.: 0.005 min
Response: 1612256792
Conc: 468.48 ng/ml

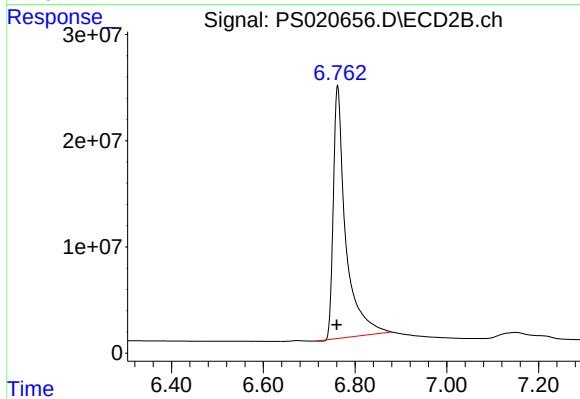

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: 0.002 min
Response: 447623241
Conc: 525.57 ng/ml

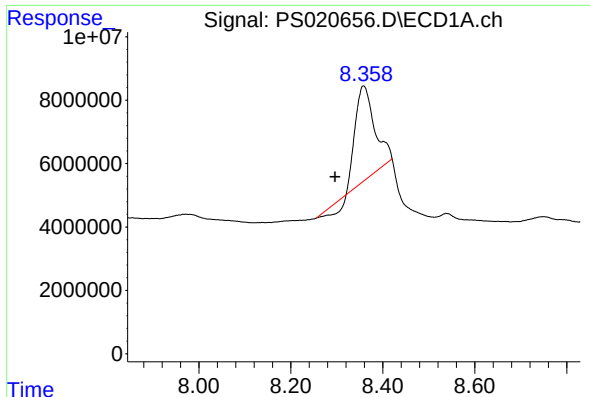

#9 2,4-D


R.T.: 8.358 min
Delta R.T.: 0.062 min
Response: 82182710
Conc: 17.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

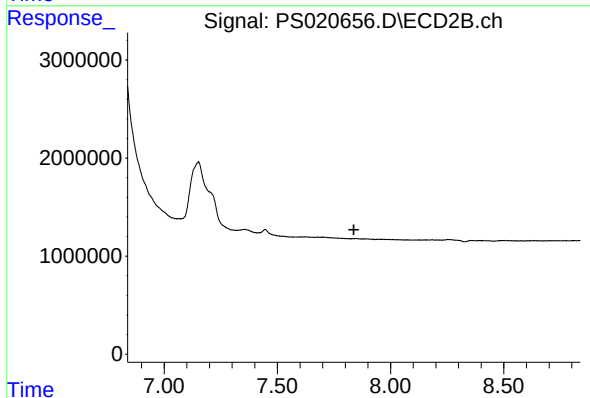


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

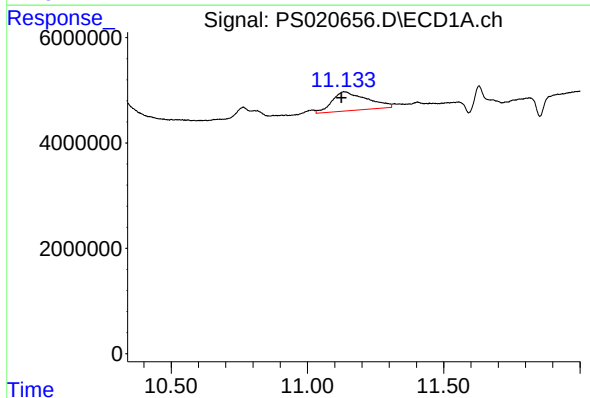

#14 DINOSEB

R.T.: 11.135 min
Delta R.T.: 0.010 min
Response: 32163139
Conc: 1.75 ng/ml

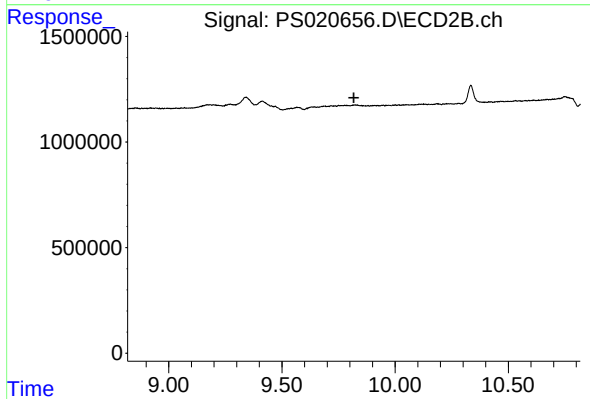

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.