

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092722\
 Data File : PD072062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2022 12:49
 Operator : AR\AJ
 Sample : PB147881BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS881

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/28/2022
 Supervised By : Ankita Jodhani 09/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:48:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.808	3.563	48652077	620.6E6	19.189	20.141
27)	SA Decachlor...	7.995	9.090	96281836	371.1E6	41.069	41.429
Target Compounds							
2)	A alpha-BHC	3.316	4.029	17768523	233.8E6	4.798	5.496
3)	MA gamma-BHC...	3.650	4.364	17700595	200.3E6	5.062	5.661
4)	MA Heptachlor	3.996	4.942	17322904	156.2E6	4.875	6.193 #
5)	MB Aldrin	4.279	5.284	17883085	134.3E6	5.032	6.111
6)	B beta-BHC	3.947	4.571	7866151	92630677	4.915m	6.226 #
7)	B delta-BHC	4.182	4.819	15005015	131.1E6	4.237	5.259
8)	B Heptachlo...	4.785	5.715	16651596	101.6E6	5.230	6.660 #
9)	A Endosulfan I	5.159	6.103	15703692	90347119	5.572	6.061
10)	B trans-Chl...	5.037	5.971	16920542	99992974	5.181	5.787
11)	B cis-Chlor...	5.103	6.048	16898700	96380013	5.266	5.726
12)	B 4,4'-DDE	5.293	6.221	29444189	175.5E6	9.948	11.698
13)	MA Dieldrin	5.426	6.381	32910116	186.5E6	10.704	12.352
14)	MA Endrin	5.702	6.614	28171213	143.7E6	10.626	11.656
15)	B Endosulfa...	5.997	6.840	27820924	149.9E6	11.148	12.338
16)	A 4,4'-DDD	5.850	6.745	25486545	140.0E6	10.917	12.117
17)	MA 4,4'-DDT	6.104	7.057	24999941	139.2E6	10.434	12.231
18)	B Endrin al...	6.178	6.971	22155413	114.9E6	10.203	11.083
19)	B Endosulfa...	6.402	7.204	26087215	128.1E6	10.337	11.117
20)	A Methoxychlor	6.683	7.533	73437649	320.3E6	57.143	61.620
21)	B Endrin ke...	6.912	7.696	32886853	156.1E6	11.629	12.500

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092722\
Data File : PD072062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2022 12:49
Operator : AR\AJ
Sample : PB147881BS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:48:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

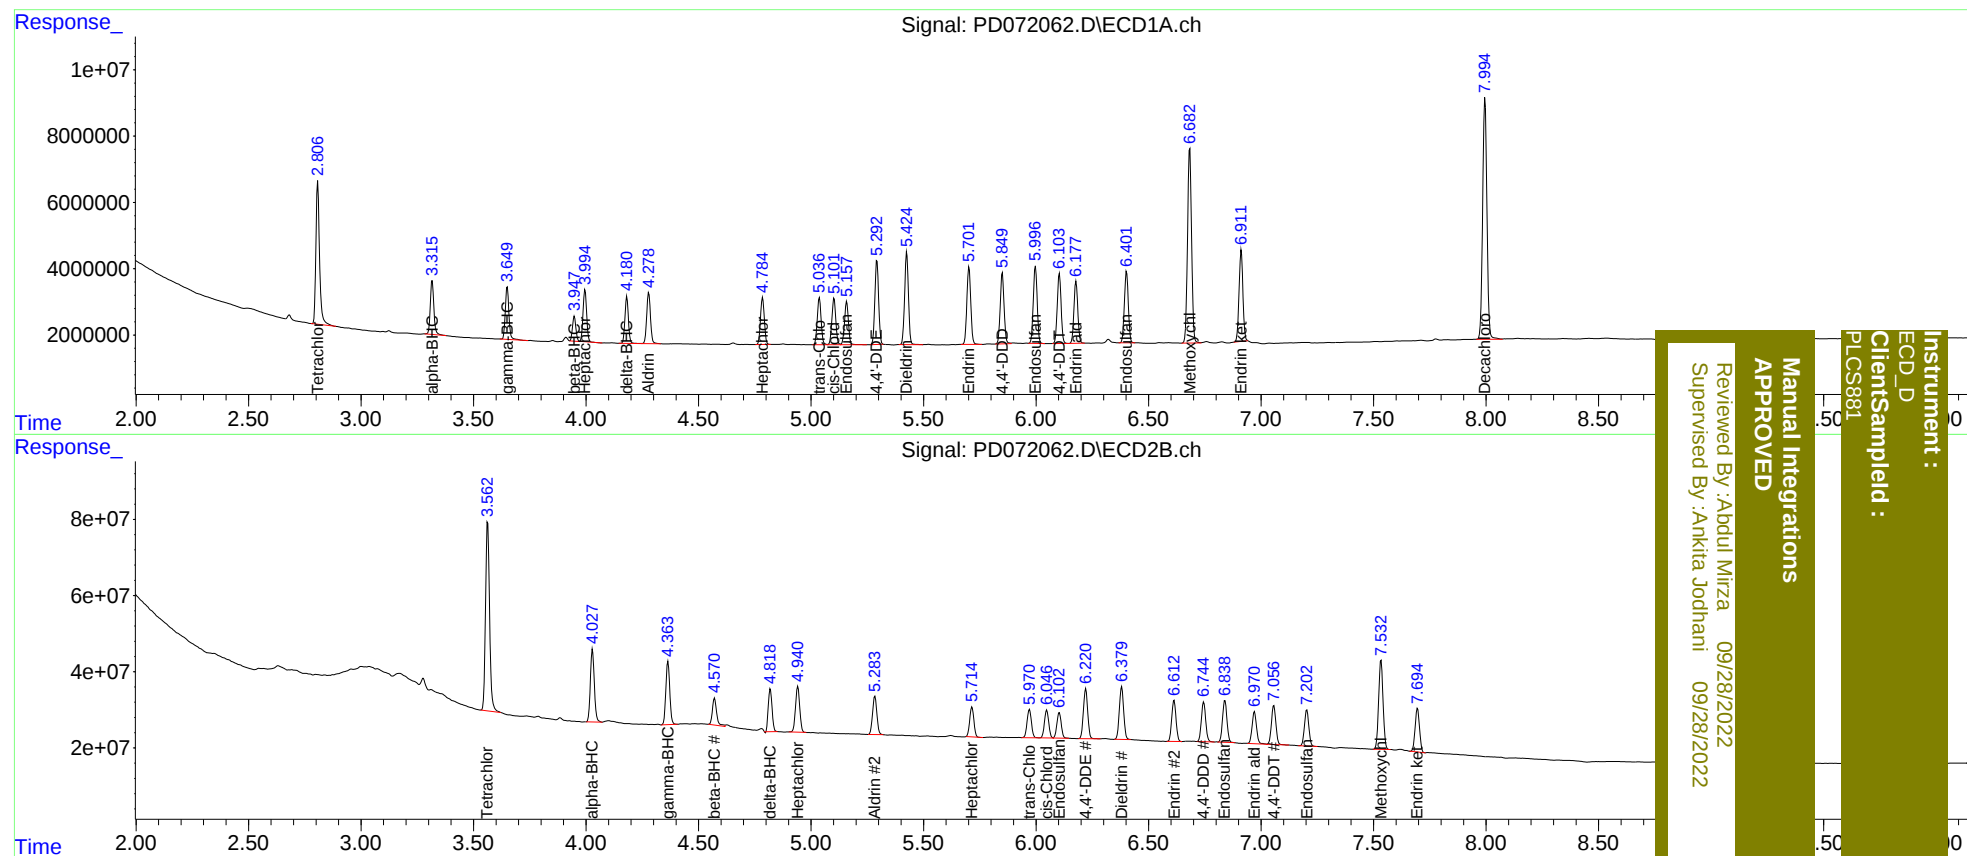

Reviewed By: Abdul Mirza 09/28/2022
Supervised By: Ankita Jodhani 09/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS881