

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 11:47
 Operator : AR\AJ
 Sample : 04480-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:37:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.758	49715189	33619315	19.591	22.748
2) SA Decachlor...	9.079	7.895	60242131	34762362	19.284	21.465
Target Compounds						
6) B beta-BHC	0.000	3.843f	0	245357	N.D.	0.248
7) B delta-BHC	0.000	4.068f	0	231052	N.D.	0.104


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 11:47
Operator : AR\AJ
Sample : 04480-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:37:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

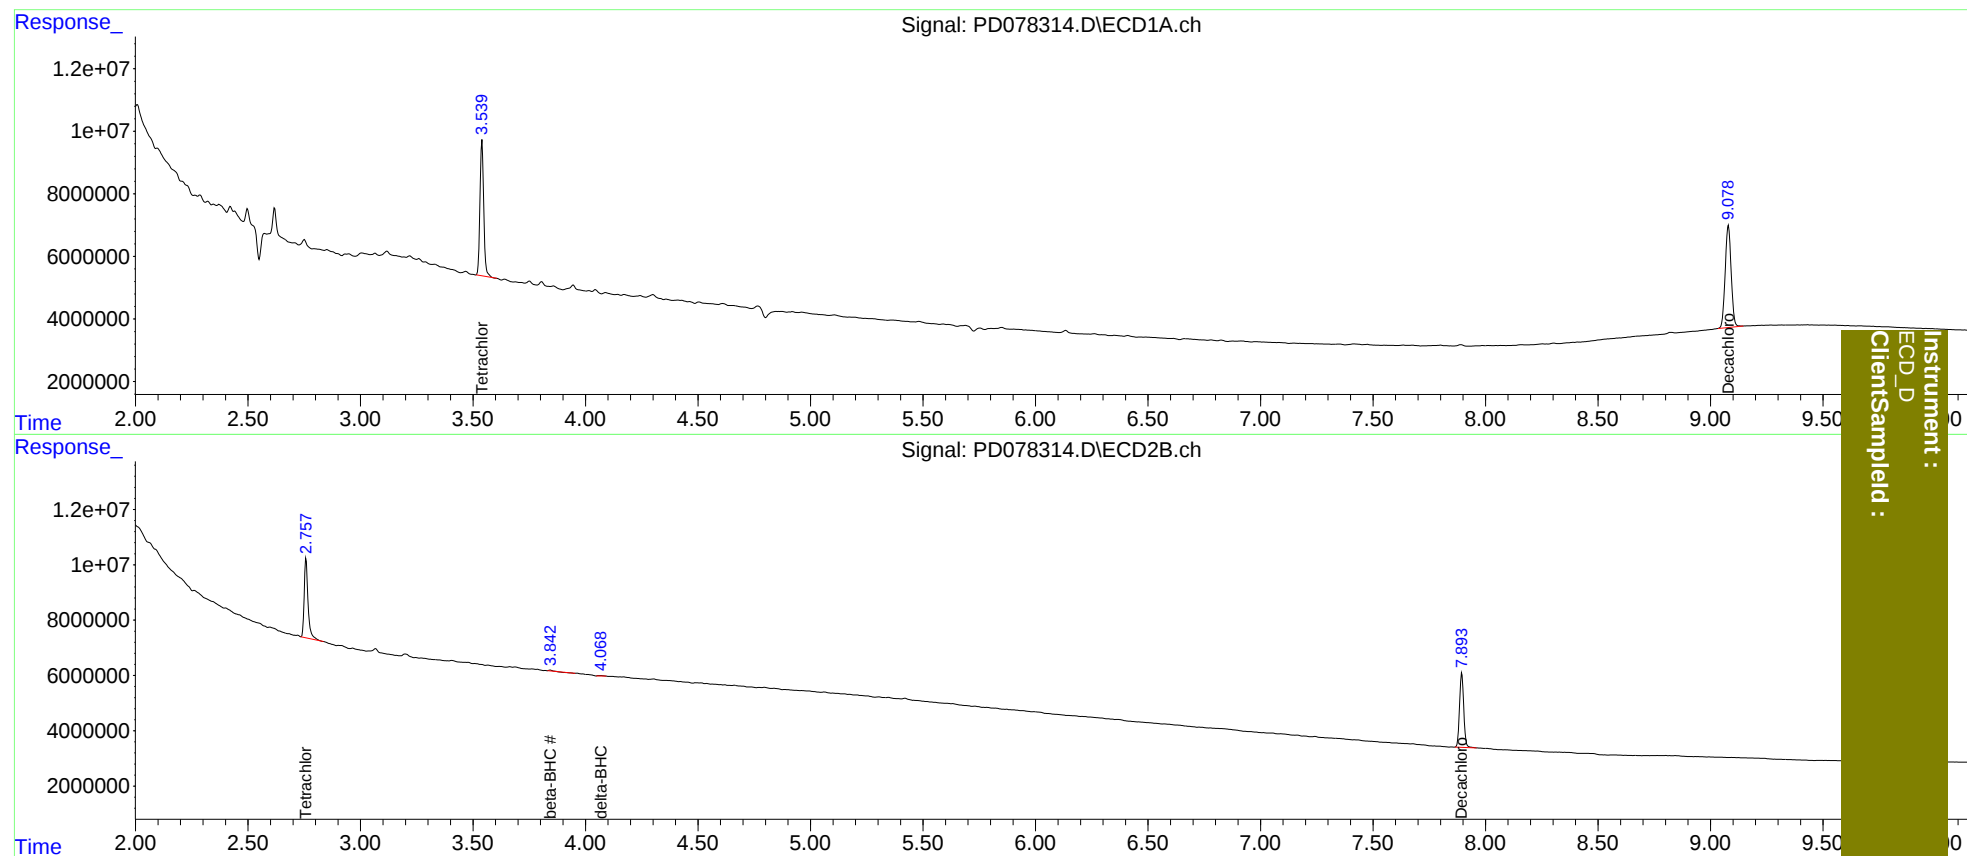


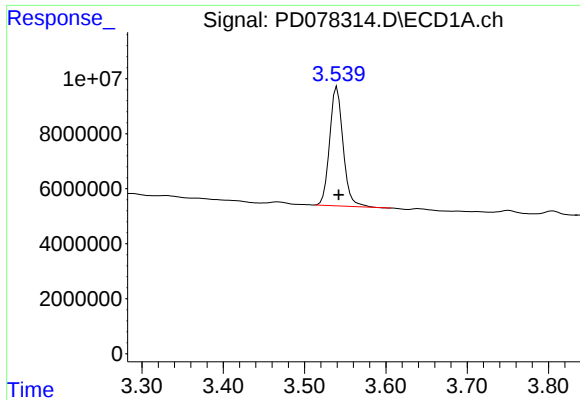

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 49715189
Conc: 19.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

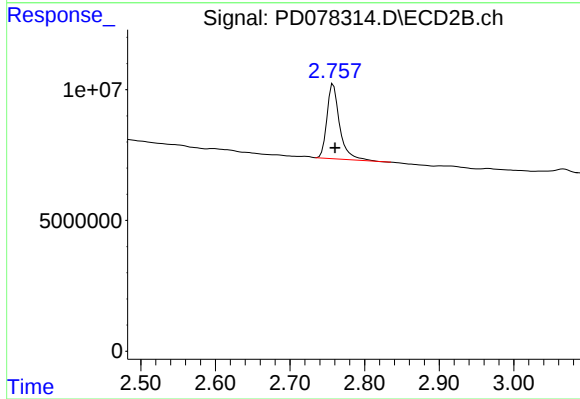


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.003 min
Response: 33619315
Conc: 22.75 ng/ml

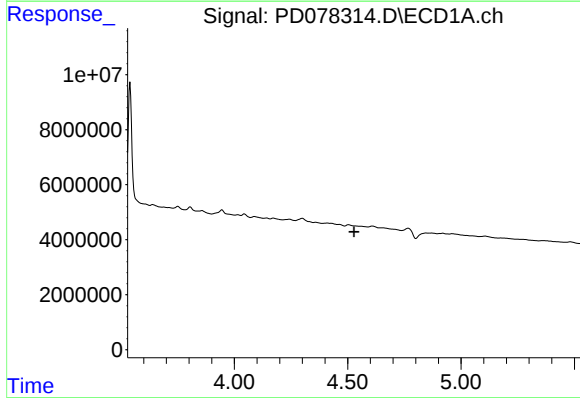


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

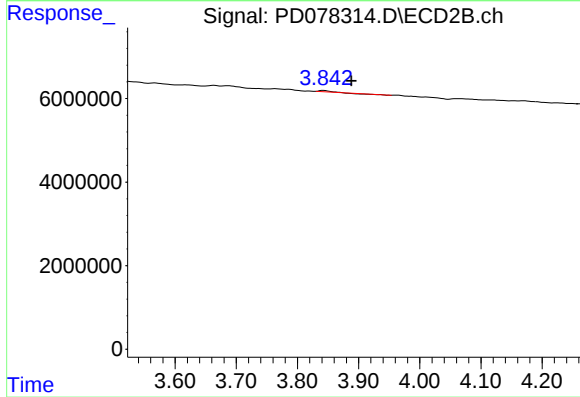

#6 beta-BHC


R.T.: 3.843 min
Delta R.T.: -0.045 min
Response: 245357
Conc: 0.25 ng/ml

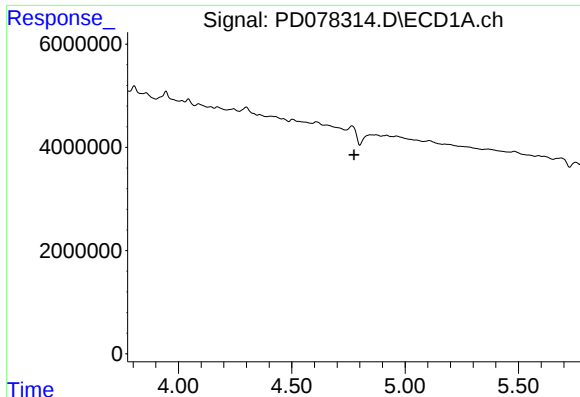

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

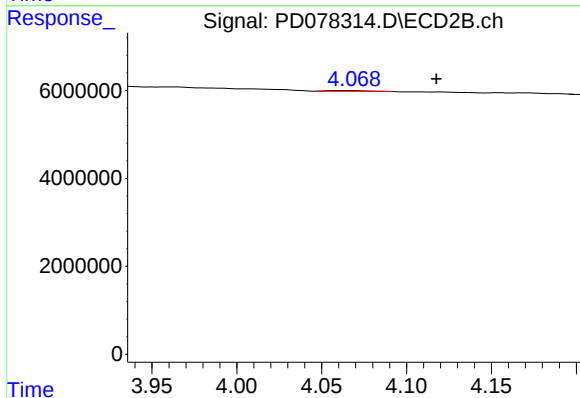


#7 delta-BHC

R.T.: 4.068 min
Delta R.T.: -0.049 min
Response: 231052
Conc: 0.10 ng/ml

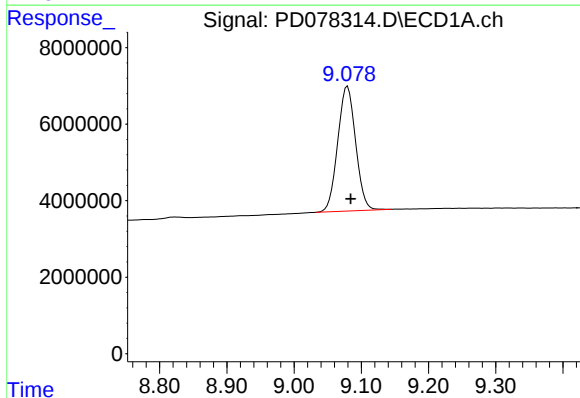

#27 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: -0.005 min
Response: 60242131
Conc: 19.28 ng/ml

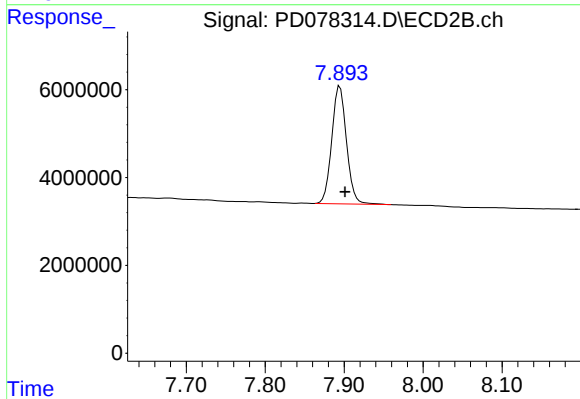

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.006 min
Response: 34762362
Conc: 21.46 ng/ml