

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 12:13
 Operator : AR\AJ
 Sample : 04480-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:38:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.759	54530241	35130724	21.488	23.771
2)	SA Decachlor...	9.080	7.895	73333671	41415364	23.475	25.573
Target Compounds							
5)	MB Aldrin	0.000	4.179f	0	145615	N.D.	<MDL
6)	B beta-BHC	0.000	3.841f	0	430759	N.D.	0.436
7)	B delta-BHC	0.000	4.069f	0	711272	N.D.	0.319


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 12:13
Operator : AR\AJ
Sample : 04480-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:38:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

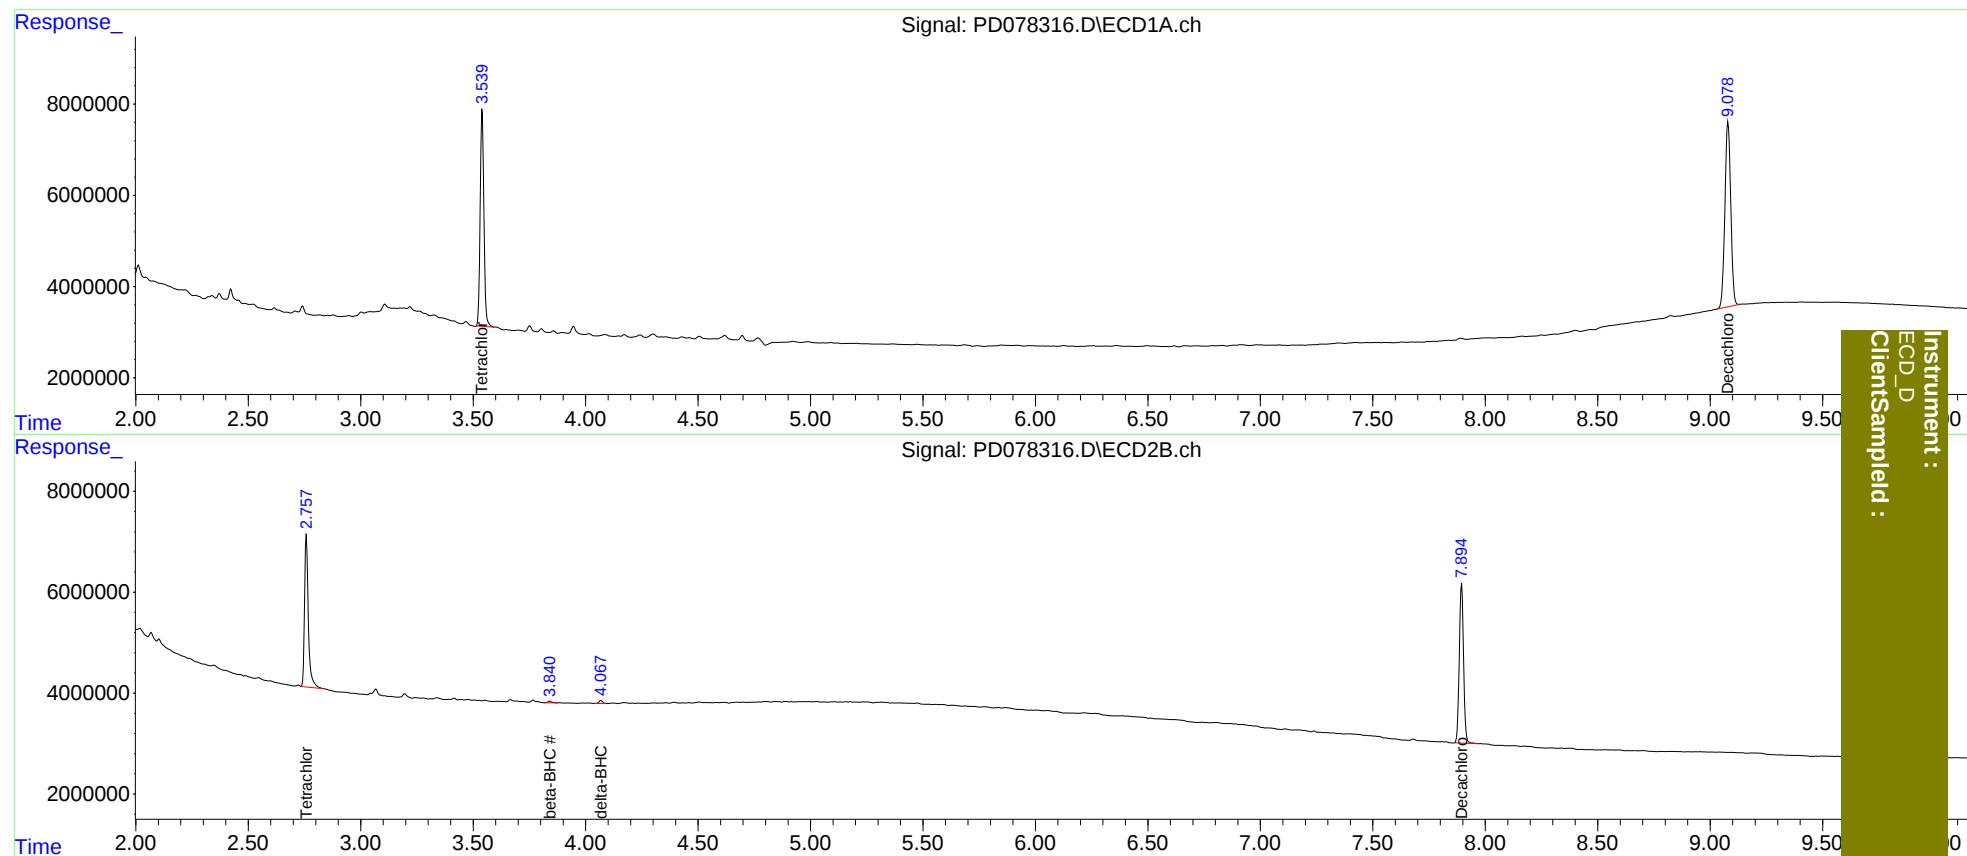


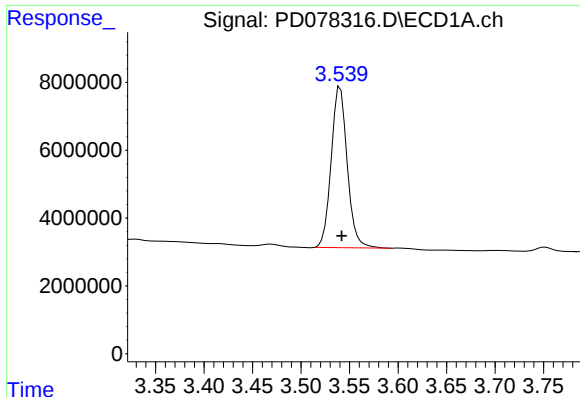

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 54530241
Conc: 21.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

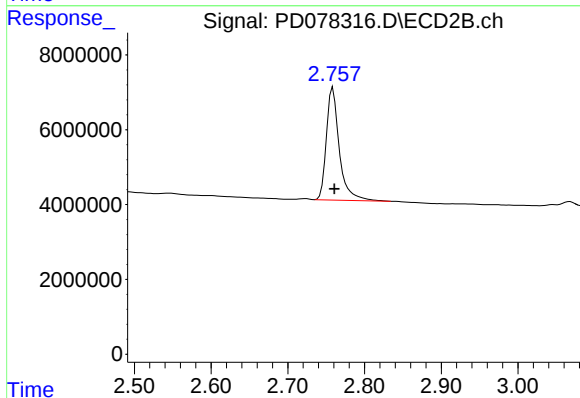


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.002 min
Response: 35130724
Conc: 23.77 ng/ml

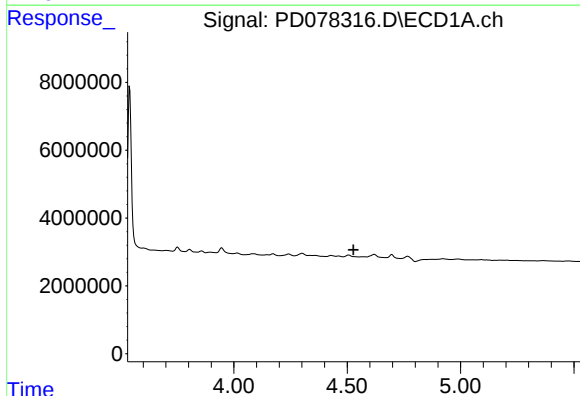


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

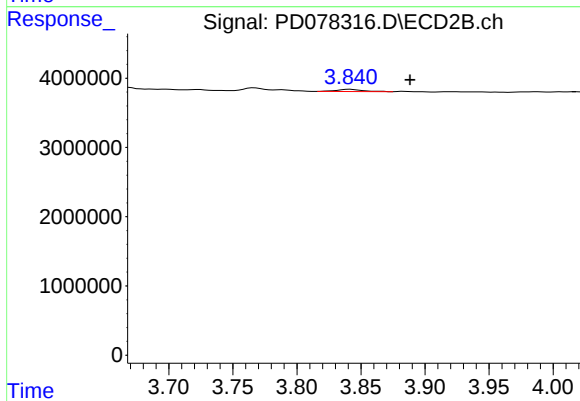

#6 beta-BHC


R.T.: 3.841 min
Delta R.T.: -0.047 min
Response: 430759
Conc: 0.44 ng/ml

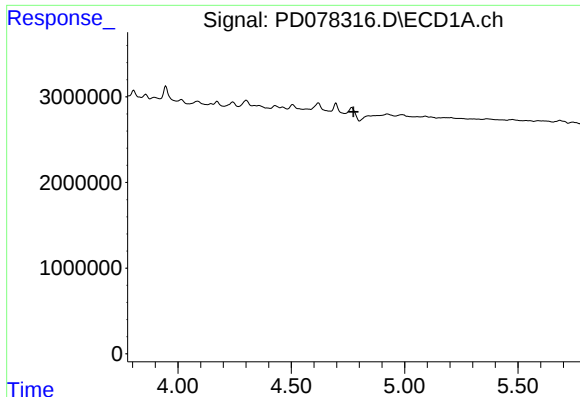

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

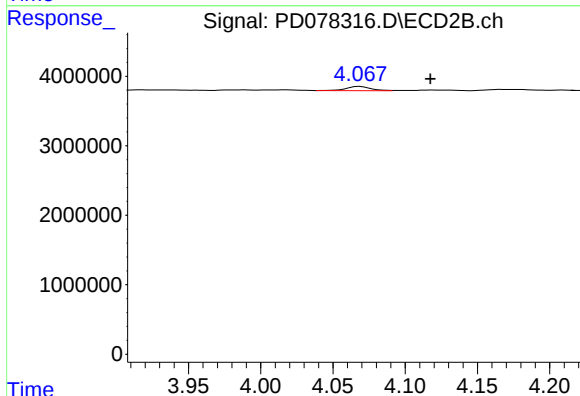


#7 delta-BHC

R.T.: 4.069 min
Delta R.T.: -0.049 min
Response: 711272
Conc: 0.32 ng/ml

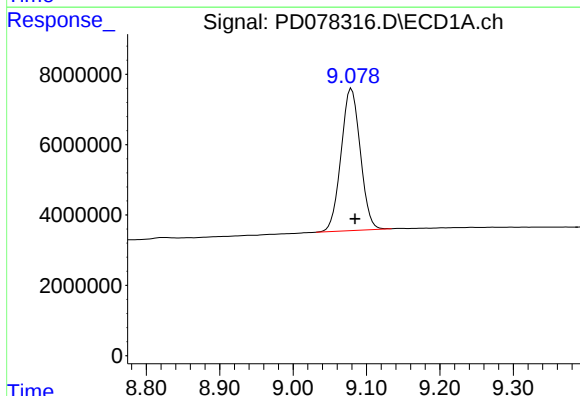

#27 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: -0.005 min
Response: 73333671
Conc: 23.48 ng/ml

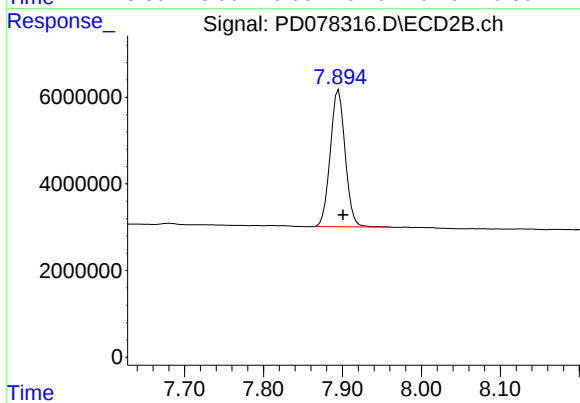

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.006 min
Response: 41415364
Conc: 25.57 ng/ml