

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 12:53
 Operator : AR\AJ
 Sample : 04480-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:39:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.758	52069562	34523902	20.518	23.360
27)	SA Decachlor...	9.080	7.895	66859096	38697038	21.402	23.894
Target Compounds							
2)	A alpha-BHC	4.029f	3.277	2235378	199166	0.522	<MDL #
3)	MA gamma-BHC...	4.290f	0.000	2843618	0	0.703	N.D. #
4)	MA Heptachlor	0.000	3.967f	0	88490	N.D.	<MDL
5)	MB Aldrin	0.000	4.191	0	209225	N.D.	<MDL
6)	B beta-BHC	0.000	3.843f	0	497424	N.D.	0.503
7)	B delta-BHC	0.000	4.147f	0	220328	N.D.	<MDL
9)	A Endosulfan I	0.000	5.100	0	241739	N.D.	0.135
10)	B trans-Chl...	0.000	4.981	0	183917	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.031	0	297136	N.D.	0.145
22)	Toxaphene-1	0.000	4.981	0	183917	N.D.	17.620


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 12:53
Operator : AR\AJ
Sample : 04480-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:39:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

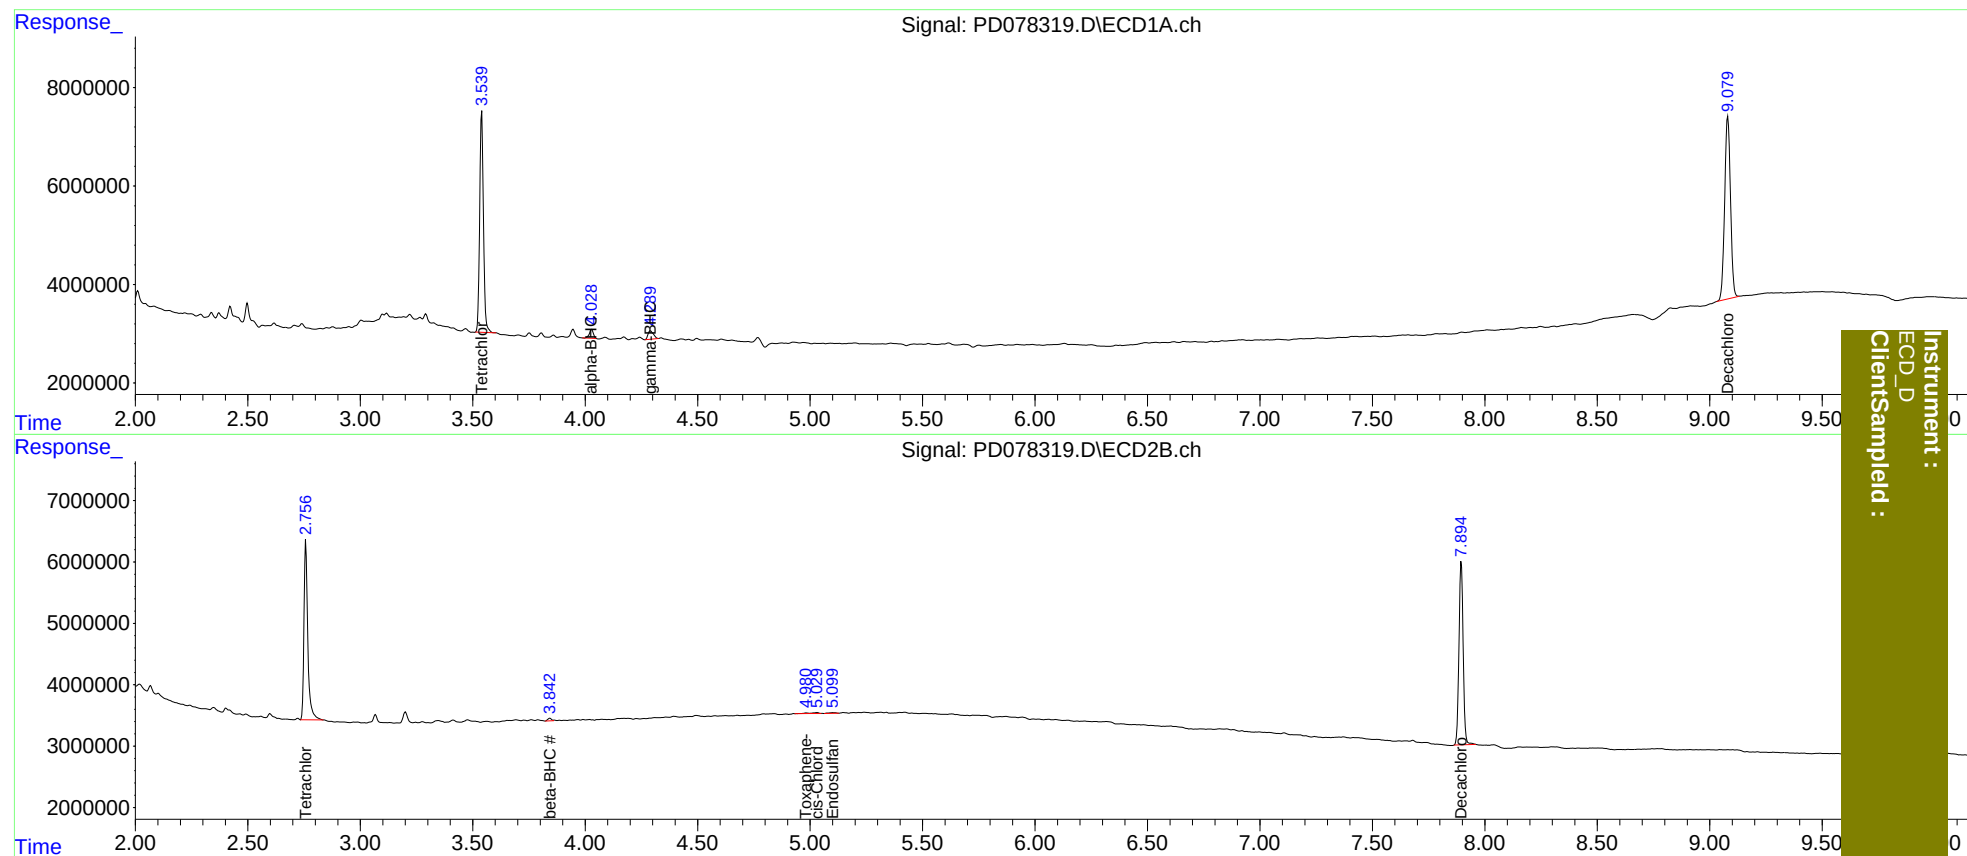


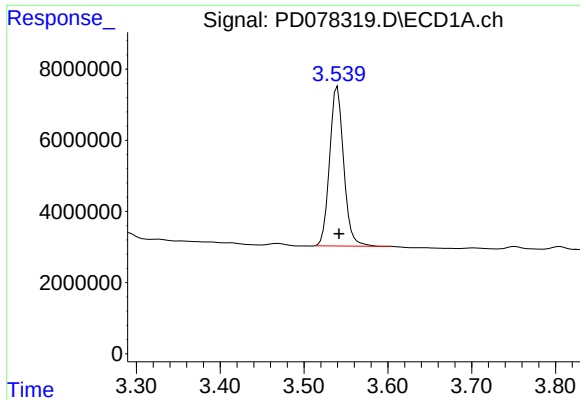

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 52069562
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

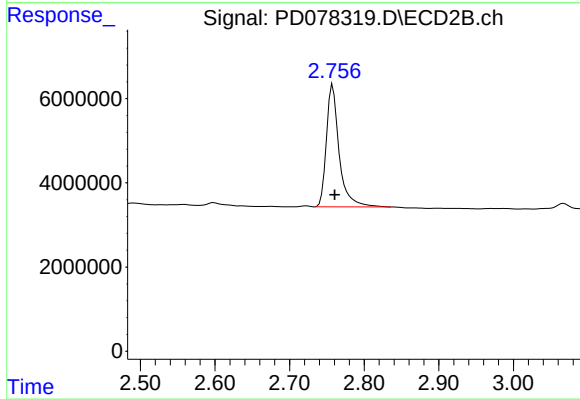


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.003 min
Response: 34523902
Conc: 23.36 ng/ml

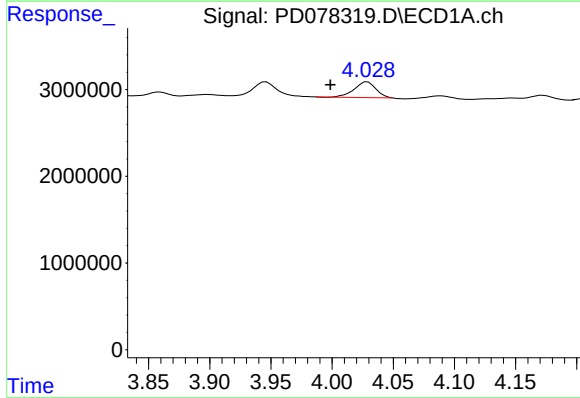


#2 alpha-BHC

R.T.: 4.029 min
Delta R.T.: 0.030 min
Response: 2235378
Conc: 0.52 ng/ml

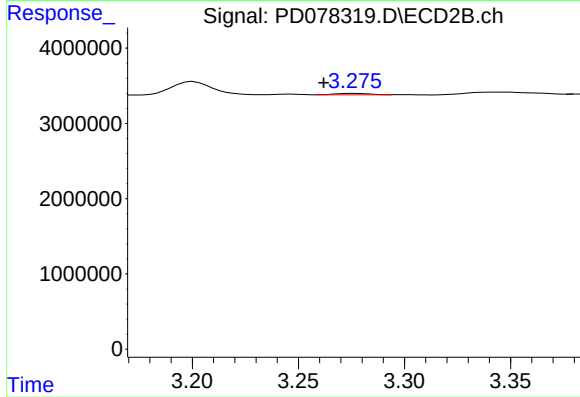

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.015 min
Response: 199166
Conc: N.D.

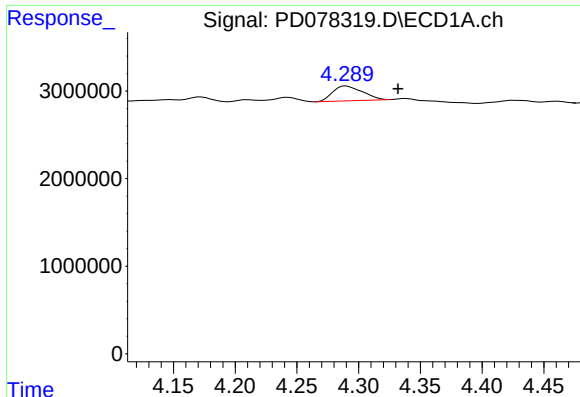

#3 gamma-BHC (Lindane)


R.T.: 4.290 min
Delta R.T.: -0.042 min
Response: 2843618
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

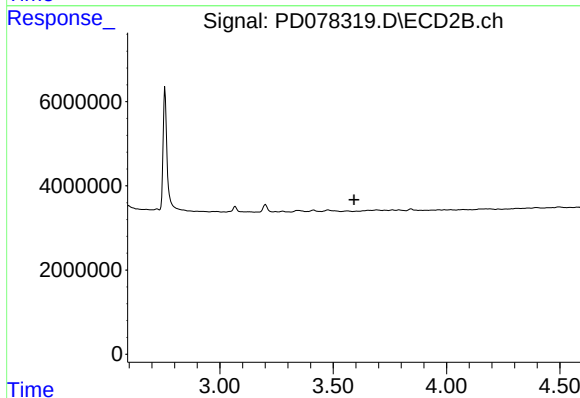


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.592 min
Response: 0
Conc: N.D.

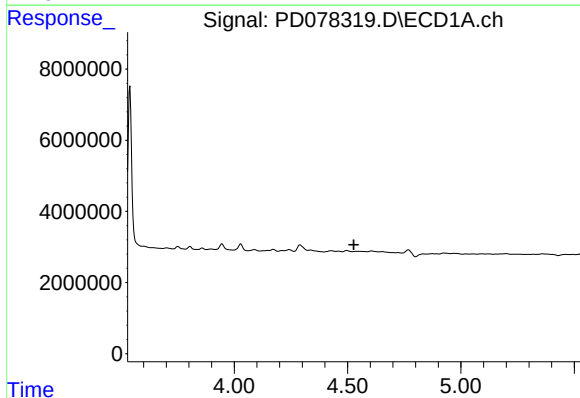


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

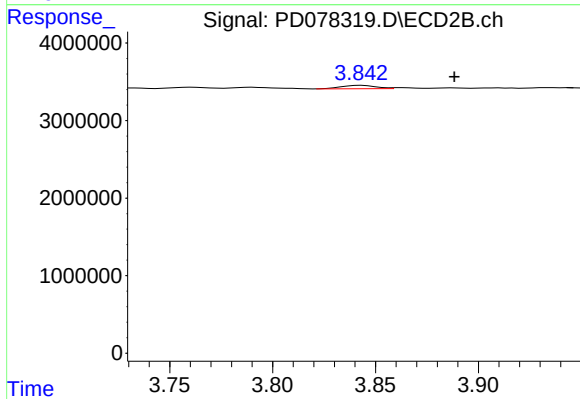

#6 beta-BHC


R.T.: 3.843 min
Delta R.T.: -0.045 min
Response: 497424
Conc: 0.50 ng/ml

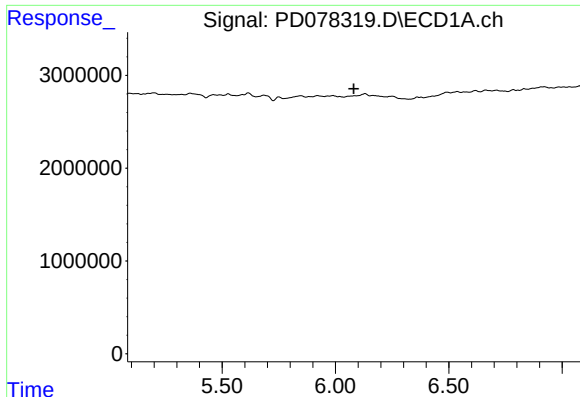

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

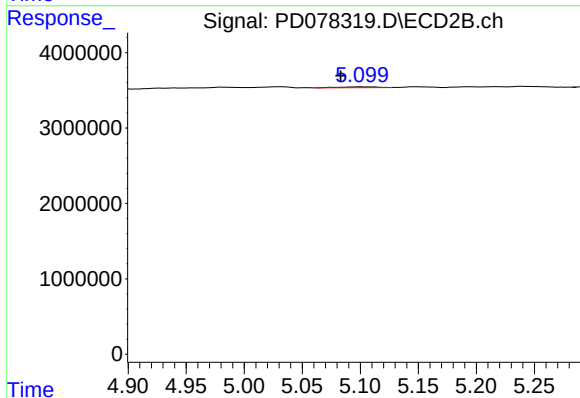


#9 Endosulfan I

R.T.: 5.100 min
Delta R.T.: 0.017 min
Response: 241739
Conc: 0.13 ng/ml

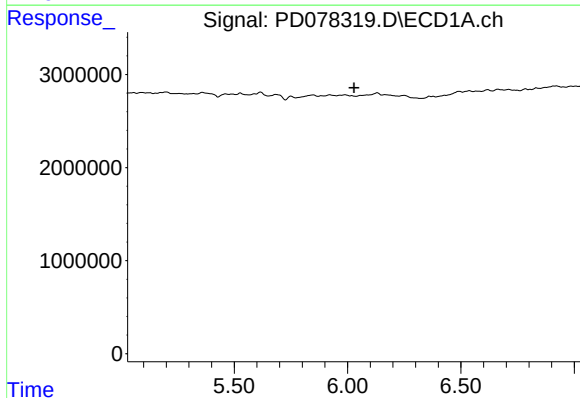


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.029 min
Response: 0
Conc: N.D.

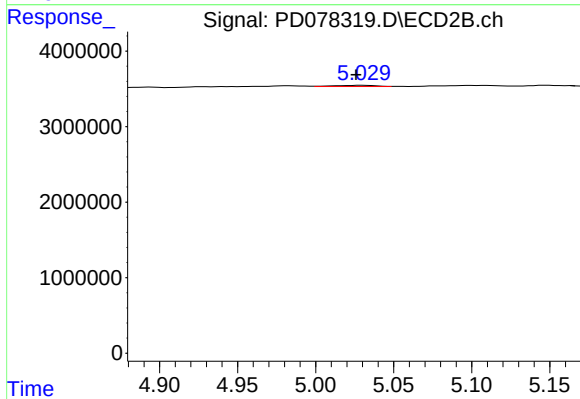

#11 cis-Chlordane


R.T.: 5.031 min
Delta R.T.: 0.005 min
Response: 297136
Conc: 0.15 ng/ml

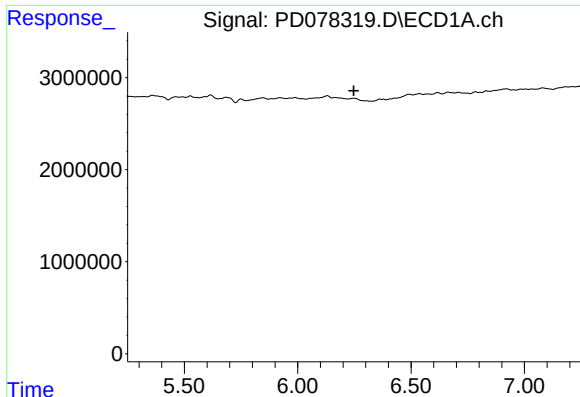

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 6.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

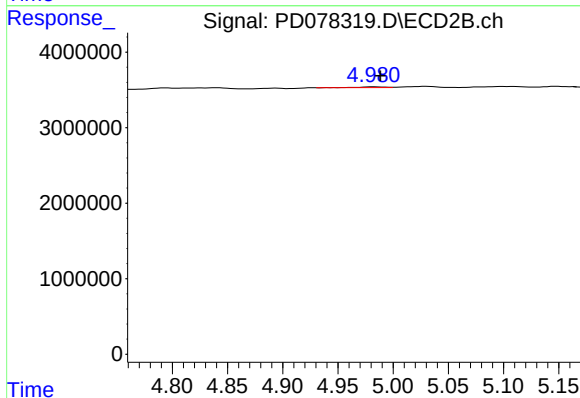


#22 Toxaphene-1

R.T.: 4.981 min
Delta R.T.: -0.007 min
Response: 183917
Conc: 17.62 ng/ml

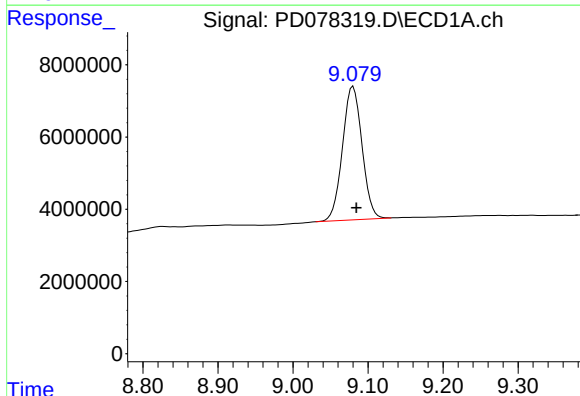

#27 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: -0.004 min
Response: 66859096
Conc: 21.40 ng/ml

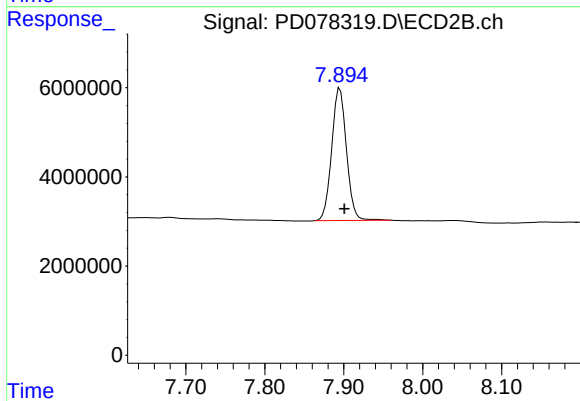

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.006 min
Response: 38697038
Conc: 23.89 ng/ml