

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 16:28
 Operator : AR\AJ
 Sample : 04480-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:45:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.758	48270469	32060675	19.021	21.694
27)	SA Decachlor...	9.077	7.893	58488555	33117264	18.723	20.449
Target Compounds							
2)	A alpha-BHC	0.000	3.275	0	222652	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.555f	0	29429	N.D.	<MDL
5)	MB Aldrin	0.000	4.212	0	26302	N.D.	<MDL
6)	B beta-BHC	0.000	3.843f	0	1374364	N.D.	1.391
7)	B delta-BHC	4.768	0.000	2511441	0	0.625	N.D. #
8)	B Heptachlo...	0.000	4.672f	0	56584	N.D.	<MDL
9)	A Endosulfan I	0.000	5.111	0	172280	N.D.	<MDL
10)	B trans-Chl...	0.000	4.988	0	275234	N.D.	0.138
11)	B cis-Chlor...	0.000	4.988f	0	275234	N.D.	0.135
22)	Toxaphene-1	0.000	4.988	0	275234	N.D.	26.369


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 16:28
Operator : AR\AJ
Sample : 04480-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:45:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

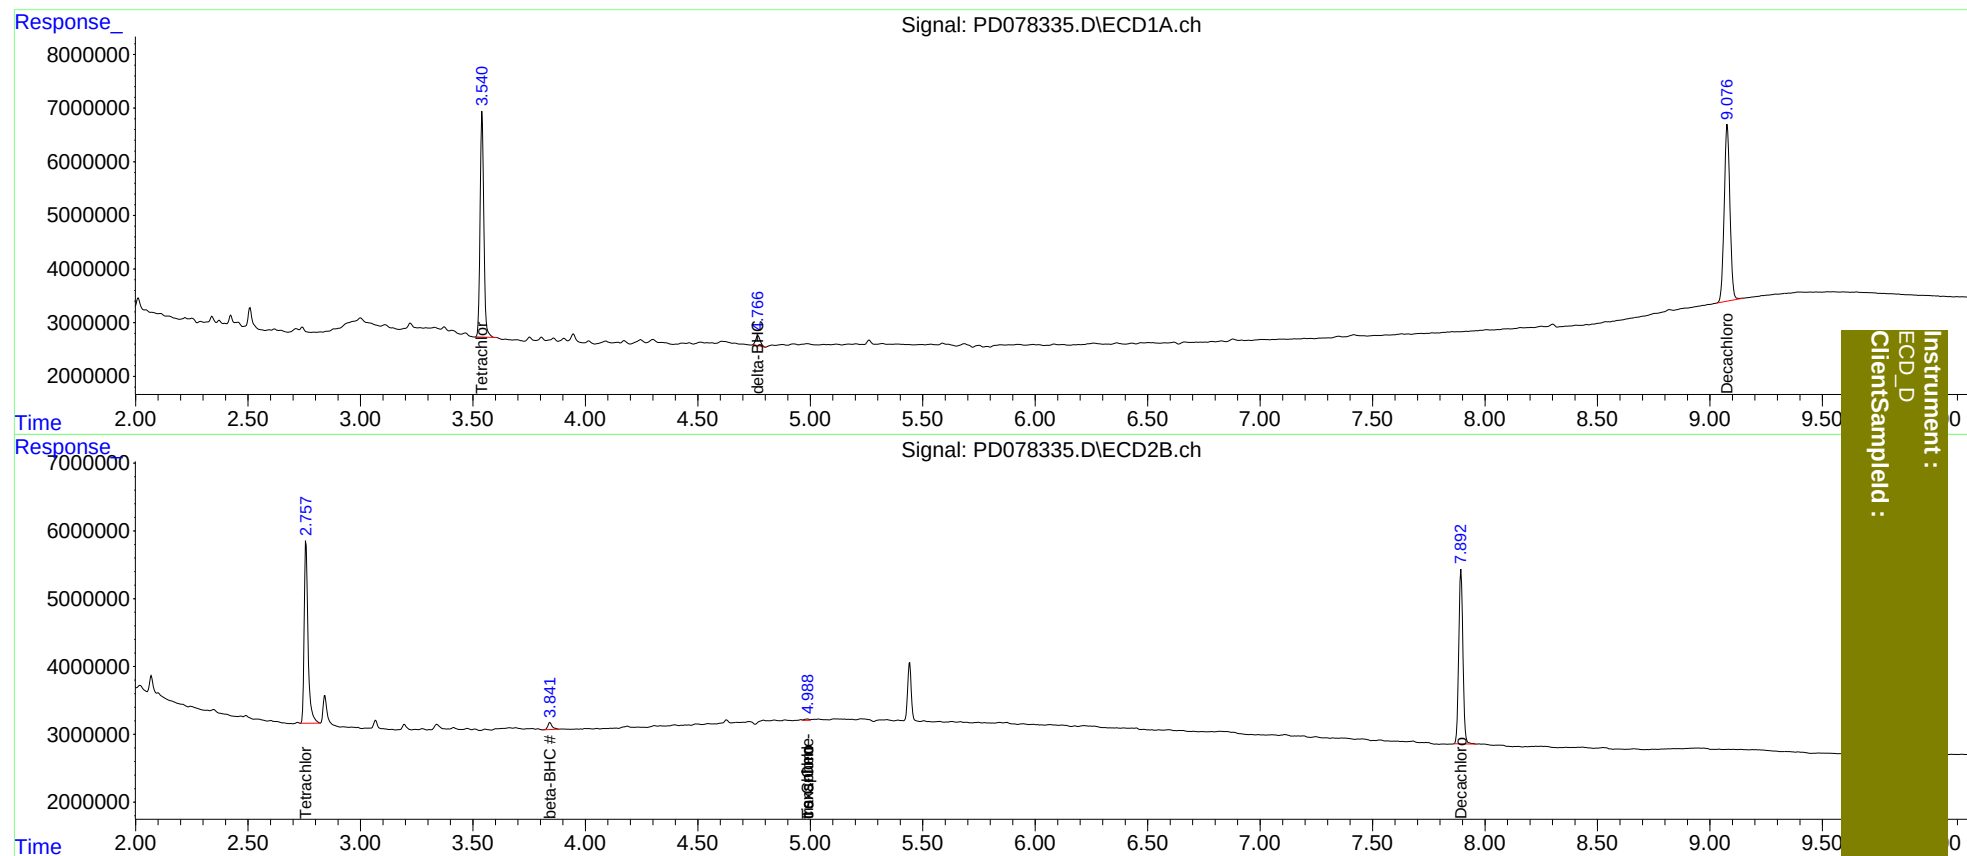


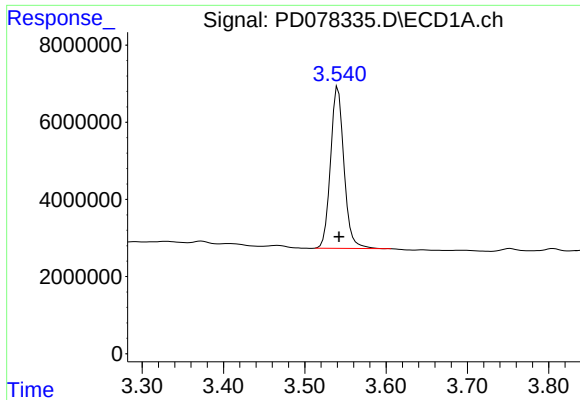

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.001 min
Response: 48270469
Conc: 19.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

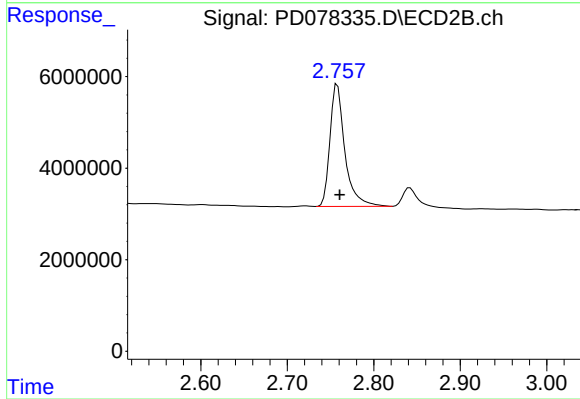


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.003 min
Response: 32060675
Conc: 21.69 ng/ml

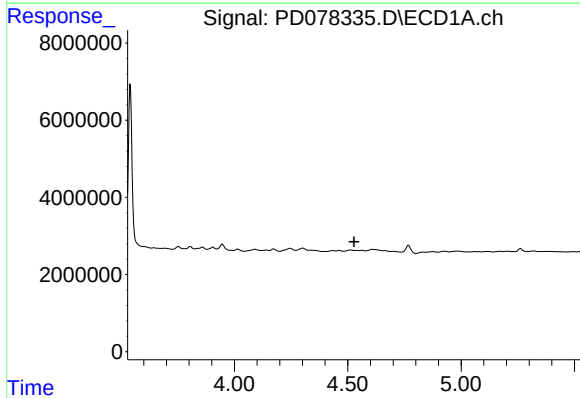


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

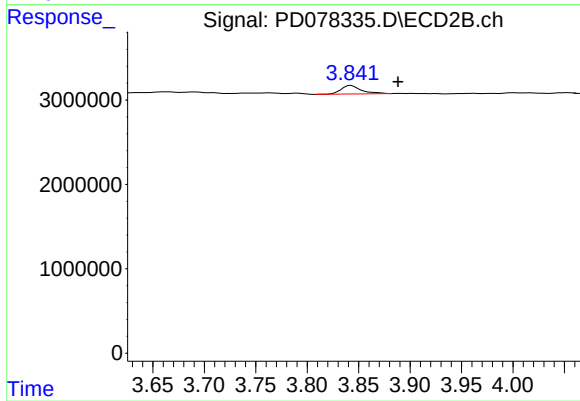

#6 beta-BHC


R.T.: 3.843 min
Delta R.T.: -0.046 min
Response: 1374364
Conc: 1.39 ng/ml

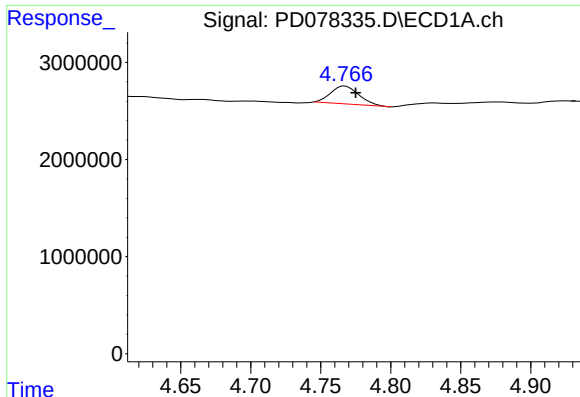

#7 delta-BHC


R.T.: 4.768 min
Delta R.T.: -0.007 min
Response: 2511441
Conc: 0.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

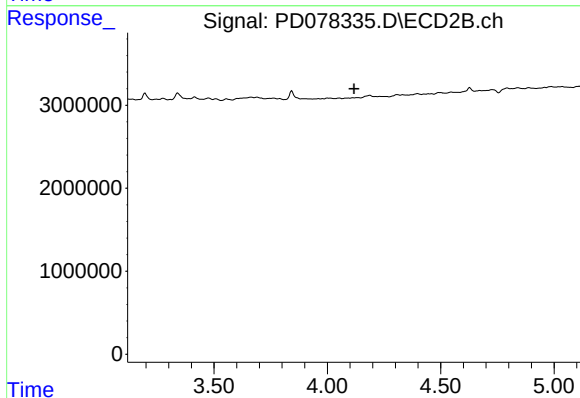


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.118 min
Response: 0
Conc: N.D.

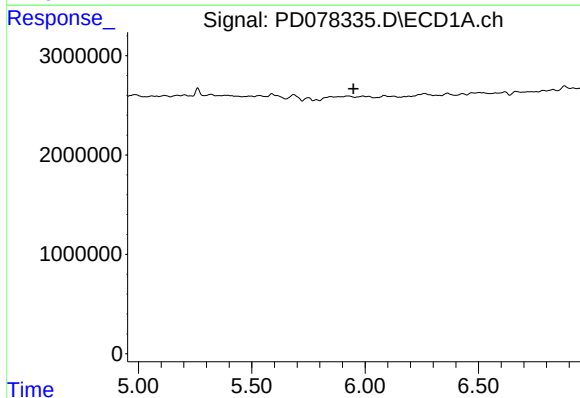


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

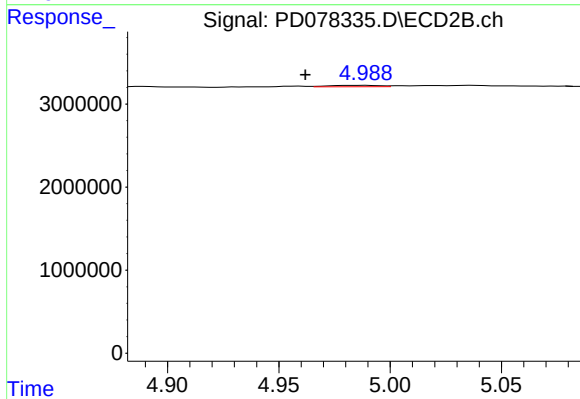

#10 trans-Chlordane

R.T.: 4.988 min
Delta R.T.: 0.026 min
Response: 275234
Conc: 0.14 ng/ml

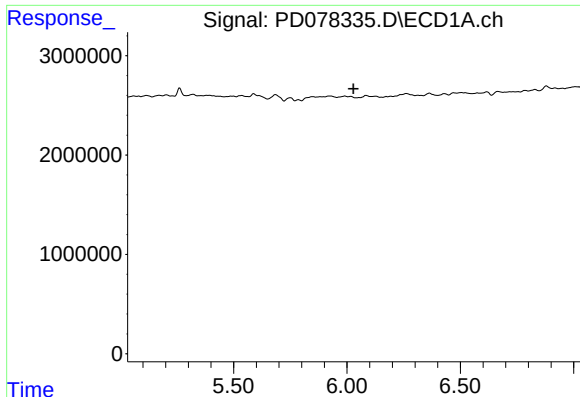

#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#11 cis-Chlordane


R.T.: 4.988 min
Delta R.T.: -0.038 min
Response: 275234
Conc: 0.13 ng/ml

#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 6.247 min
Response: 0
Conc: N.D.

#22 Toxaphene-1


R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 275234
Conc: 26.37 ng/ml

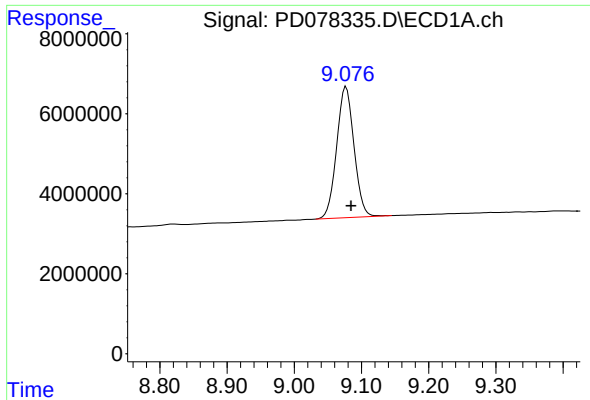

#27 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: -0.007 min
Response: 58488555
Conc: 18.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

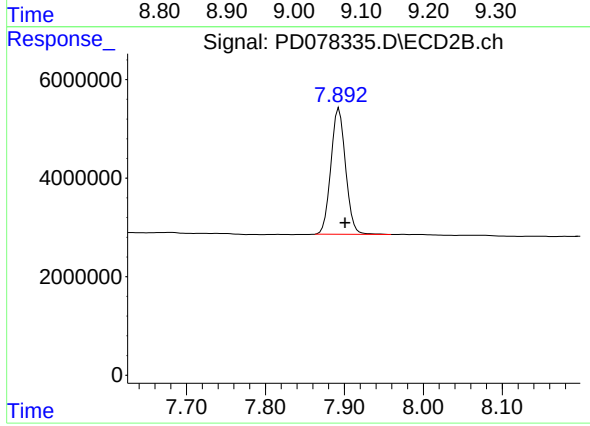

#27 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: -0.008 min
Response: 33117264
Conc: 20.45 ng/ml