

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 03:21
 Operator : AR\AJ
 Sample : PB155861BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:35:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	48835791	32165824	19.244	21.765
2)	SA Decachlor...	9.077	7.894	72309001	39363045	23.147	24.305
Target Compounds							
3)	MA gamma-BHC...	0.000	3.605	0	32878	N.D.	<MDL
4)	MA Heptachlor	0.000	3.934	0	2829	N.D.	<MDL
5)	MB Aldrin	0.000	4.223	0	92948	N.D.	<MDL
6)	B beta-BHC	0.000	3.934f	0	2829	N.D.	<MDL
7)	B delta-BHC	4.766	0.000	1414850	0	0.352	N.D. #
8)	B Heptachlo...	0.000	4.652f	0	14258	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 03:21
Operator : AR\AJ
Sample : PB155861BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:35:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

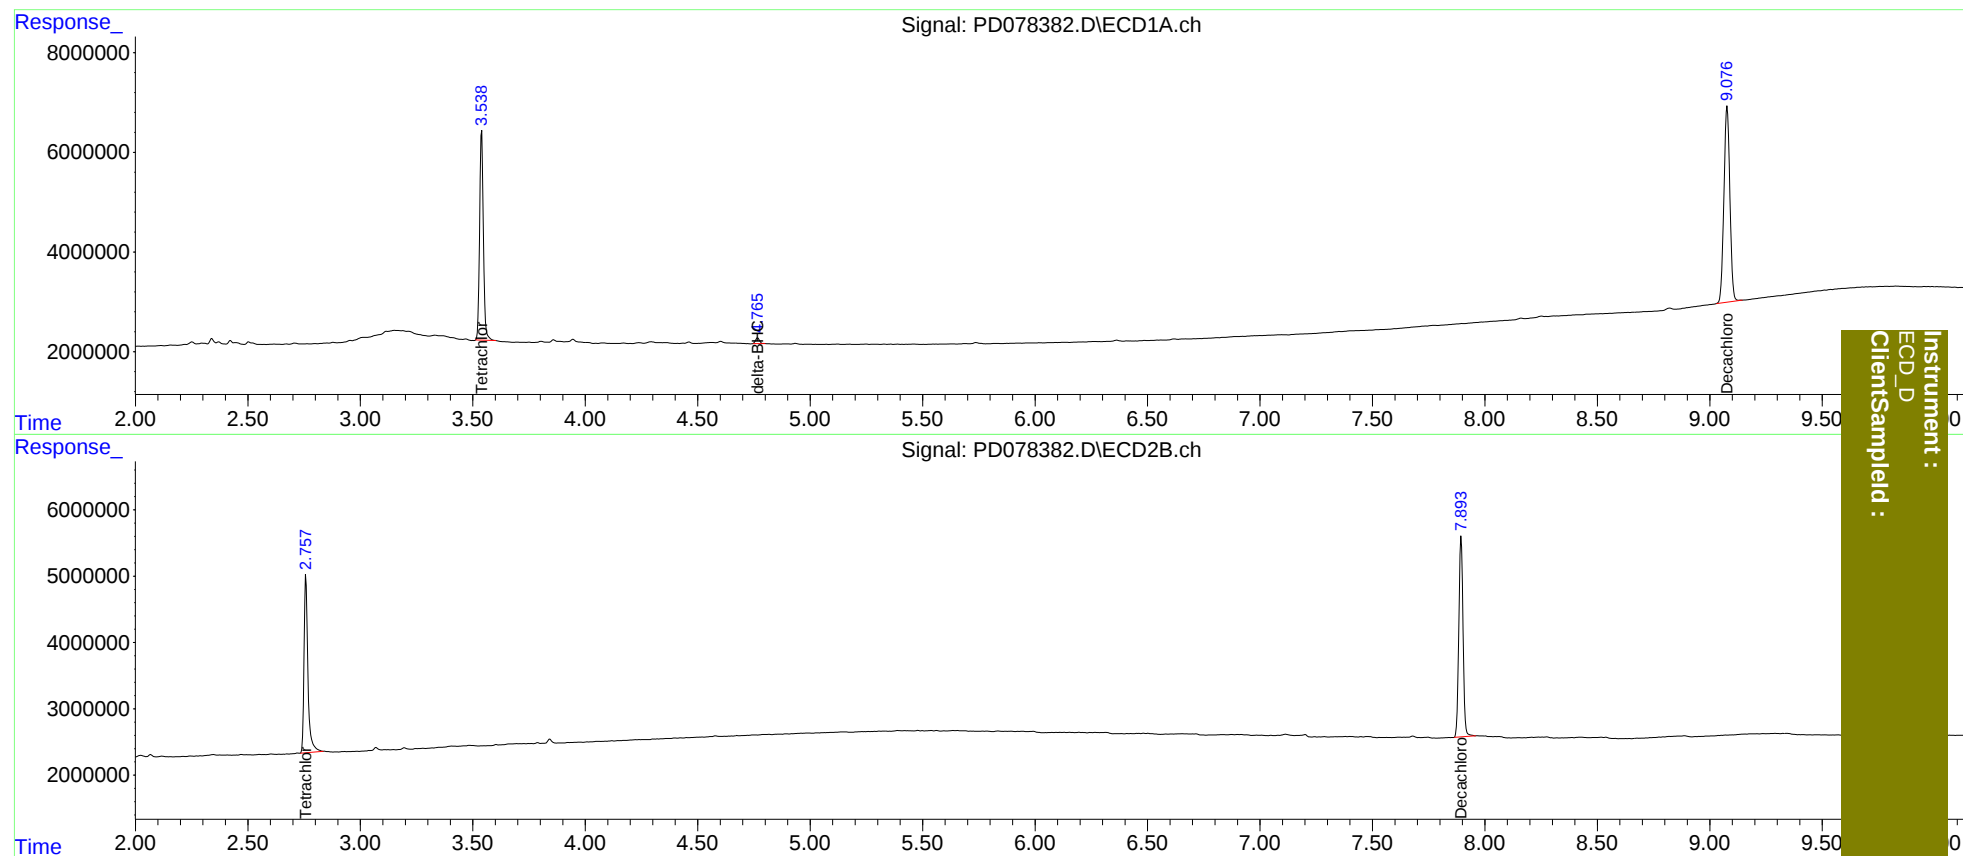


Instrument :
ECD_D
ClientSampled :
PB155861BL

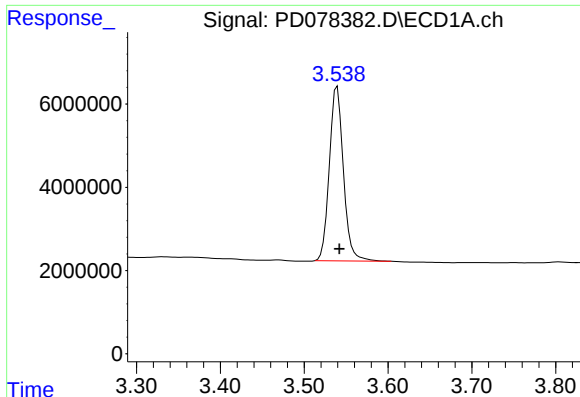

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 48835791
Conc: 19.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

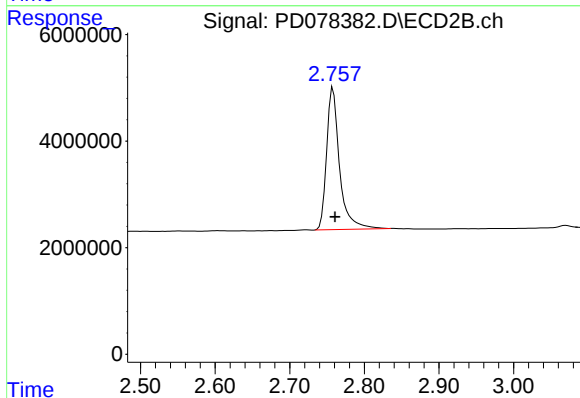


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.003 min
Response: 32165824
Conc: 21.76 ng/ml

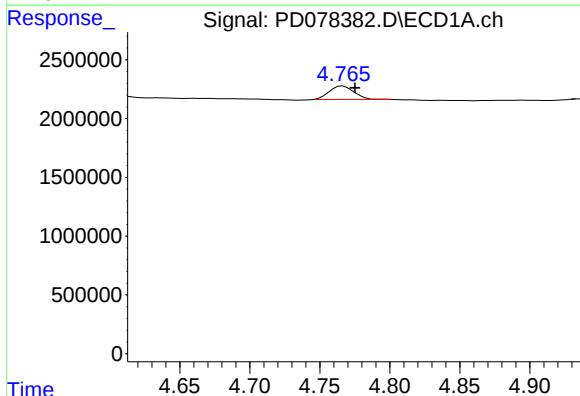


#7 delta-BHC

R.T.: 4.766 min
Delta R.T.: -0.009 min
Response: 1414850
Conc: 0.35 ng/ml

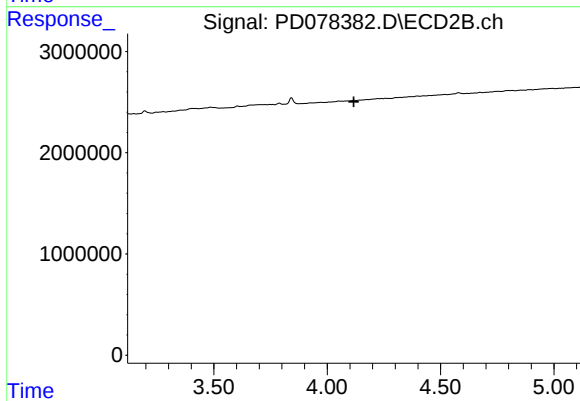

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.118 min
Response: 0
Conc: N.D.

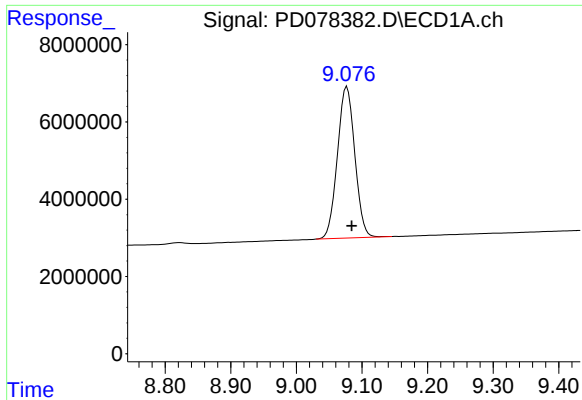

#27 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: -0.007 min
Response: 72309001
Conc: 23.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

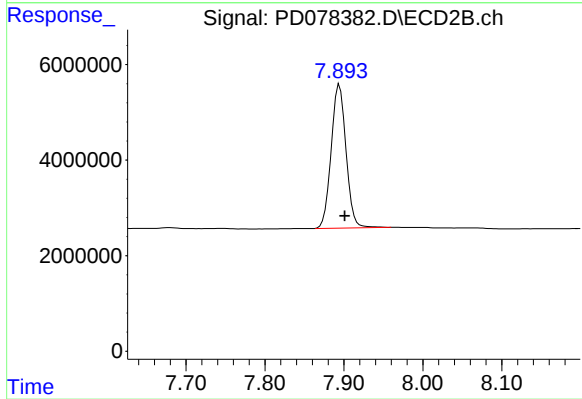

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: -0.006 min
Response: 39363045
Conc: 24.31 ng/ml