

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 09:41
 Operator : AR\AJ
 Sample : 04472-01DL 2X
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYE8DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/28/2023
 Supervised By : Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 07:03:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.759	15769786	10697230	6.214	7.238
2)	SA Decachlor...	9.084	7.896	22984104	12809538	7.357	7.909
Target Compounds							
5)	MB Aldrin	5.261	4.218	210.3E6	39147595	50.365m	17.466 #
7)	B delta-BHC	4.779	4.124	21341421	145.7E6	5.315m	65.359 #
11)	B cis-Chlor...	6.027	5.018	39815839	125.5E6	10.331m	61.381 #
19)	B Endosulfa...	7.167	6.337	2458.0E6	1832.3E6	811.150m	1108.969 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 09:41
Operator : AR\AJ
Sample : 04472-01DL 2X
Misc :
ALS Vial : 95 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 07:03:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

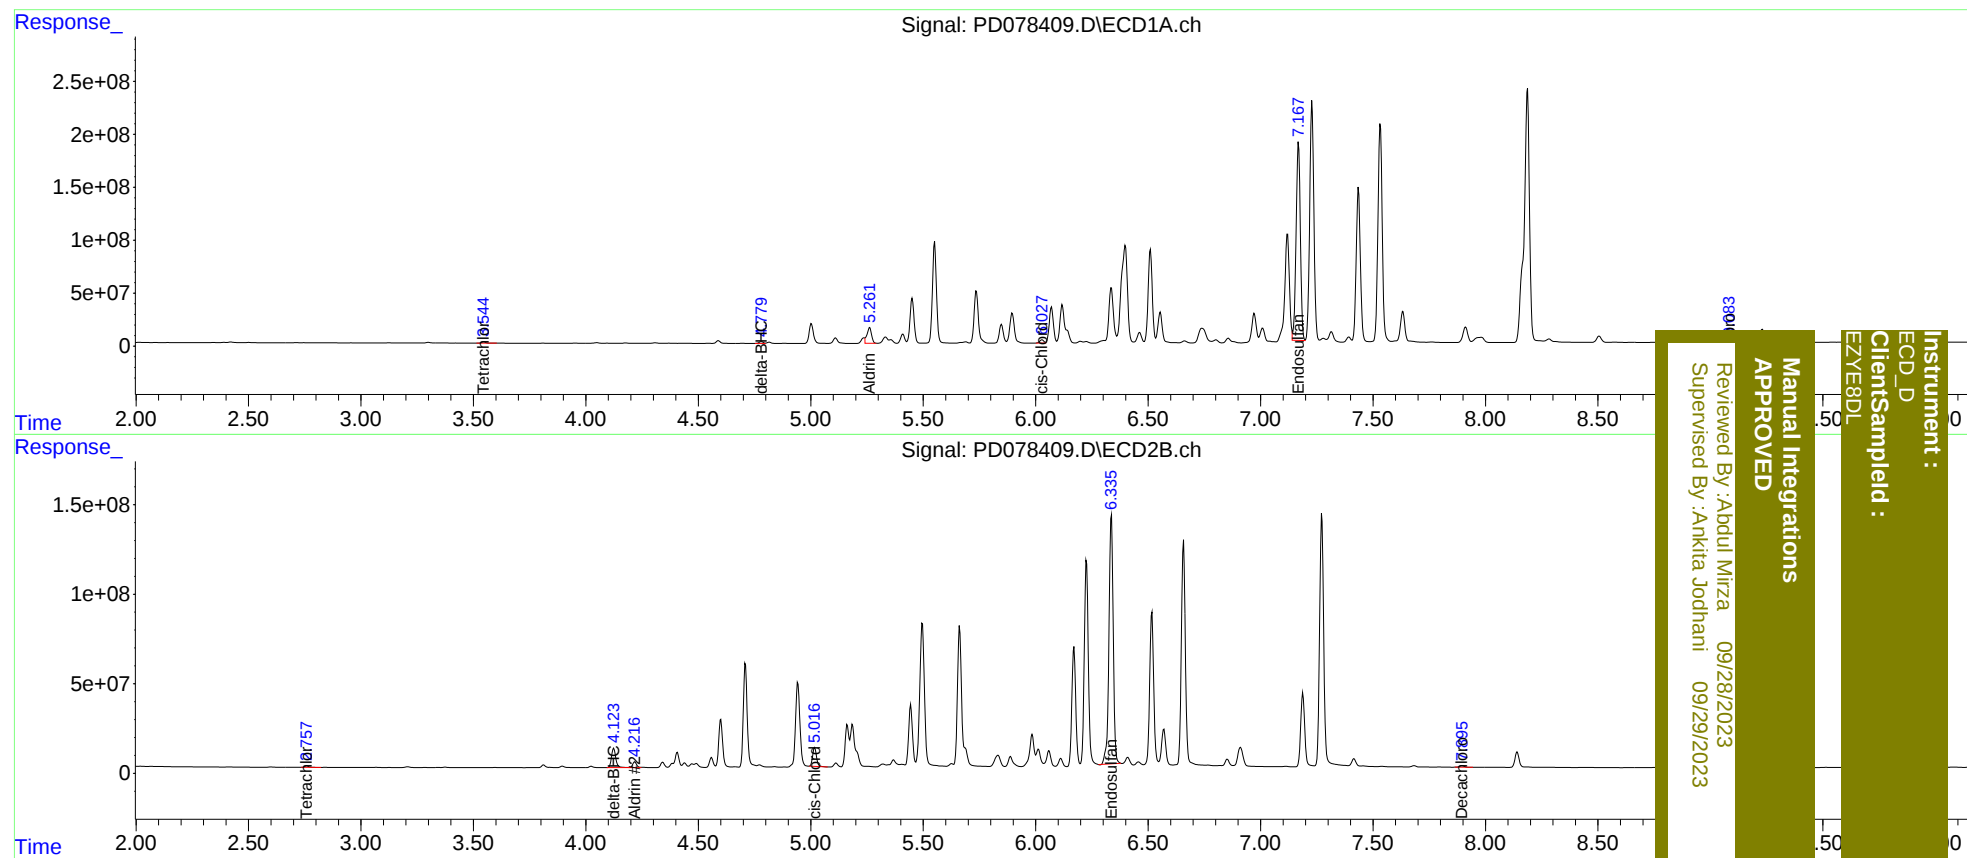

Reviewed By: Abdul Mirza 09/28/2023
Supervised By: Ankita Jodhani 09/29/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EZE8DL