

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092723\  
 Data File : PD078336.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 26 Sep 2023 16:45  
 Operator : ARVAJ  
 Sample : 04480-21  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1



**Instrument :**  
 ECD\_D  
**ClientSampleId :**  
 BBJ07

**Manual Integrations APPROVED**

Reviewed By : Abdul Mirza 09/27/2023  
 Supervised By : Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 26 21:46:01 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD090623CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Sep 06 16:40:06 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

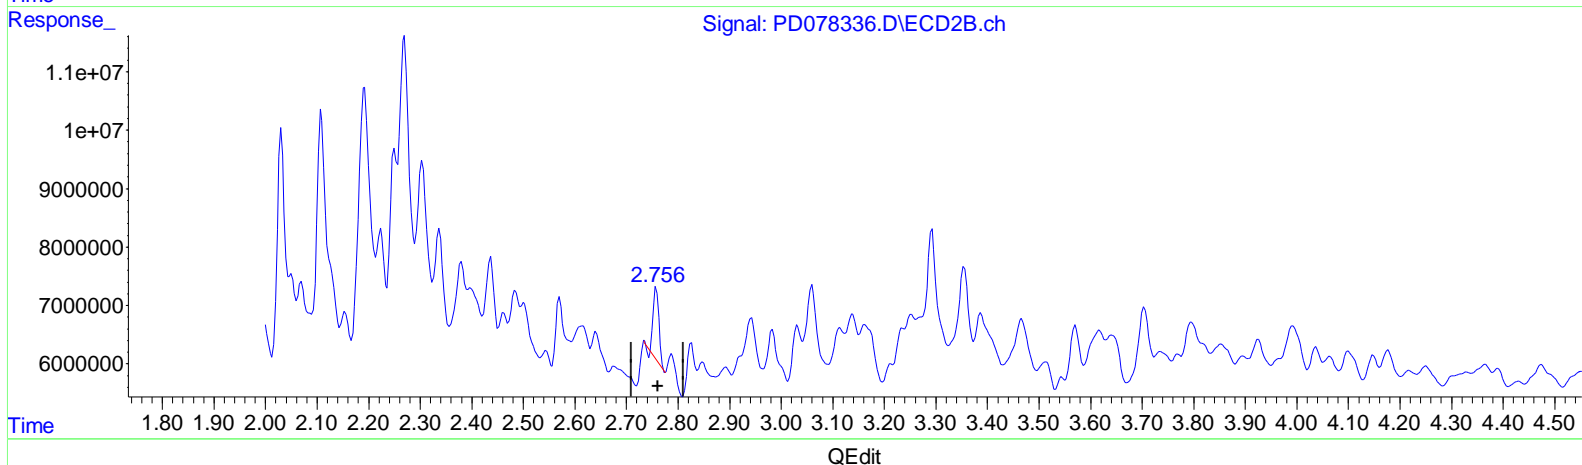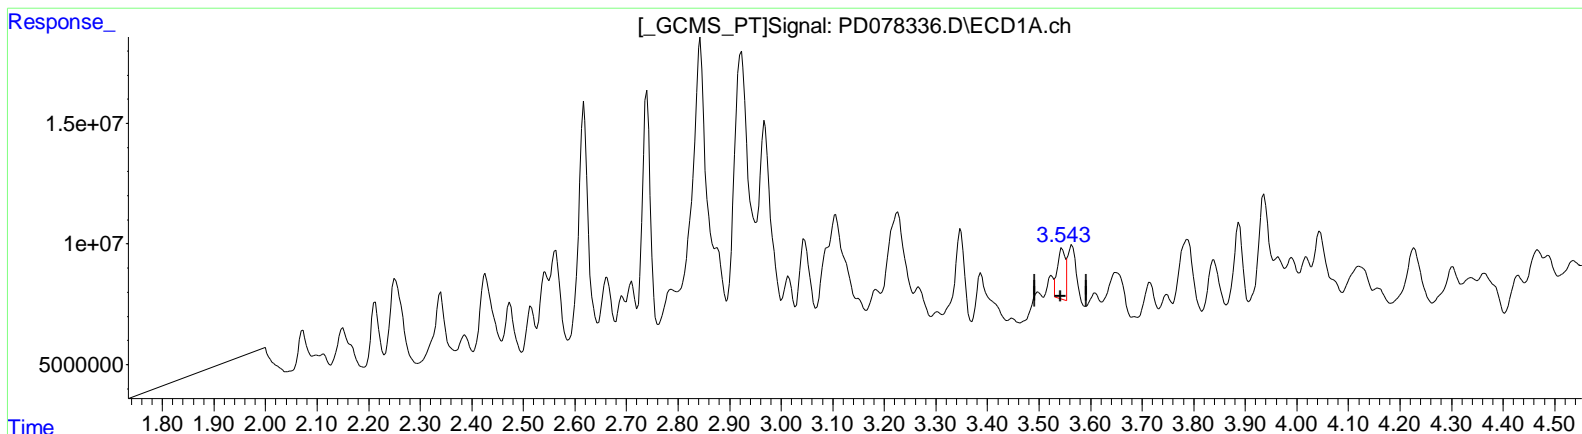

(1) Tetrachloro-m-xylene (SA)  
 3.545min 8.796 ng/ml  
 response 22321128

(1) Tetrachloro-m-xylene #2 (SA)  
 2.758min 6.646 ng/ml  
 response 9821273

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092723\  
 Data File : PD078336.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 26 Sep 2023 16:45  
 Operator : ARVAJ  
 Sample : 04480-21  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1



**Instrument :**  
 ECD\_D  
**ClientSampleId :**  
 BBJ07

**Manual Integrations APPROVED**

Reviewed By : Abdul Mirza 09/27/2023  
 Supervised By : Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 26 21:46:01 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD090623CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Sep 06 16:40:06 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

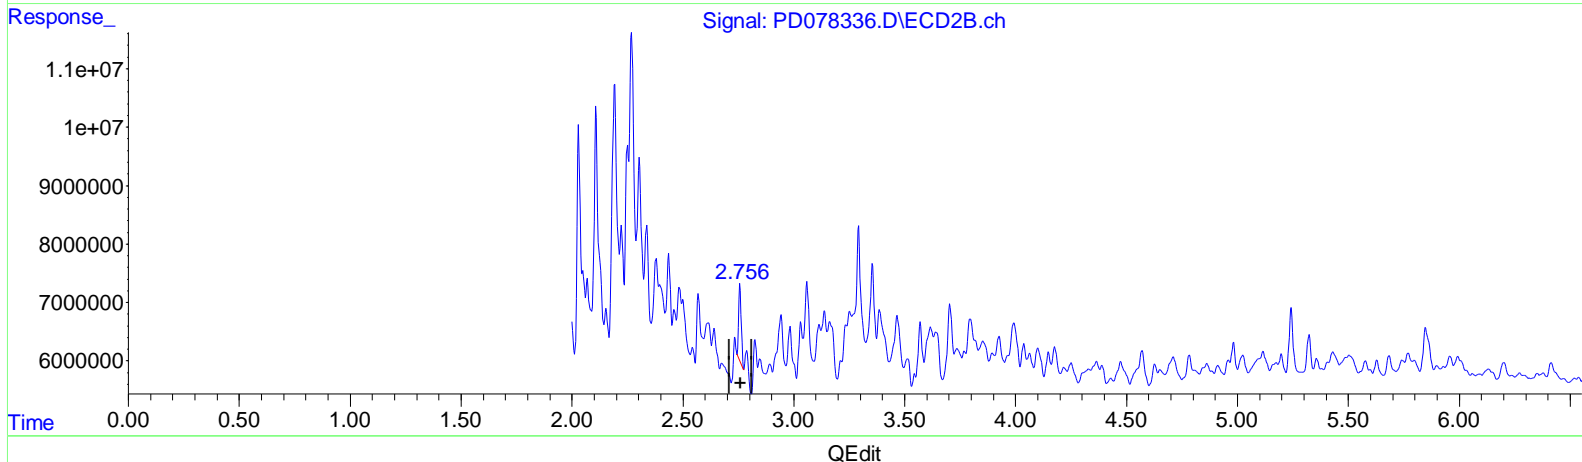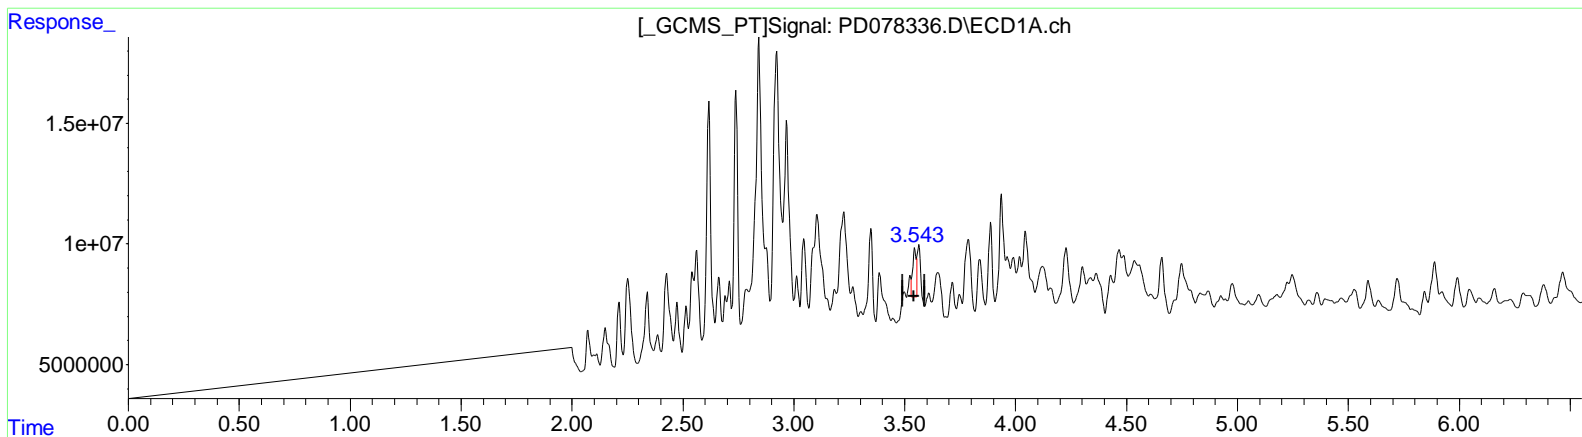

(1) Tetrachloro-m-xylene (SA)  
 3.543min 9.085 ng/ml m  
 response 23054859

(1) Tetrachloro-m-xylene #2 (SA)  
 2.756min 7.492 ng/ml m  
 response 11071866