

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
 Data File : PD078408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 09:23
 Operator : AR\AJ
 Sample : 04472-01DL2 20X
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYE8DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/28/2023
 Supervised By : Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 07:08:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.757	1493809	1093745	0.589	0.740 #
2)	SA Decachlor...	9.079	7.894	2969735	1373084	0.951	0.848
Target Compounds							
5)	MB Aldrin	5.255	4.216	25253467	4583373	6.049m	2.045 #
7)	B delta-BHC	4.773	4.122	2555877	16186533	0.637m	7.262 #
11)	B cis-Chlor...	6.024	5.016	4670905	14218513	1.212	6.953 #
19)	B Endosulfa...	7.162	6.334	239.3E6	200.7E6	78.956m	121.448 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092723\
Data File : PD078408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 09:23
Operator : AR\AJ
Sample : 04472-01DL2 20X
Misc :
ALS Vial : 94 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 07:08:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

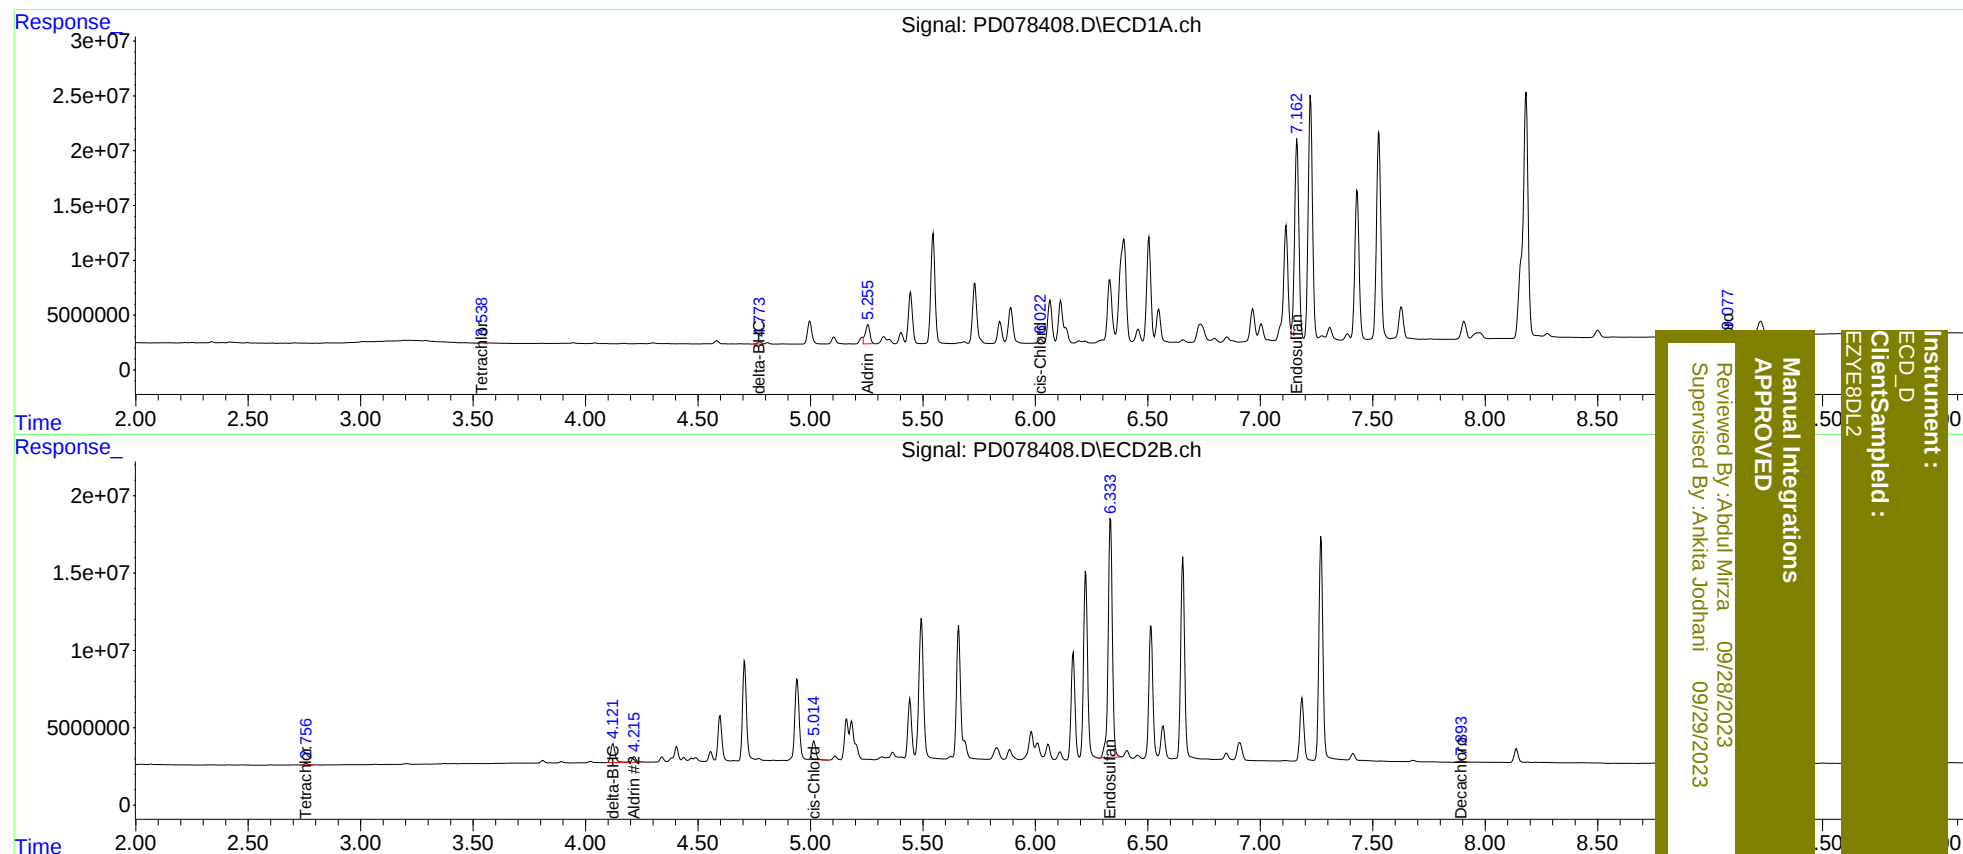

Reviewed By: Abdul Mirza 09/28/2023
Supervised By: Ankita Jodhani 09/29/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EZE8DL2