

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 17:47
 Operator : AR\AJ
 Sample : PB163566BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:15:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.879	19818517	79416445	18.917	18.757
27)	SA Decachlor...	8.886	8.063	32088293	80223164	21.768	20.748
Target Compounds							
2)	A alpha-BHC	3.931f	0.000	47306	0	<MDL	N.D. #
3)	MA gamma-BHC...	4.170f	0.000	15317116	0	8.091	N.D. #
4)	MA Heptachlor	4.842f	0.000	85009	0	<MDL	N.D. #
5)	MB Aldrin	5.164	0.000	72168	0	<MDL	N.D. #
7)	B delta-BHC	4.660	0.000	1021191	0	0.577	N.D. #
8)	B Heptachlo...	5.547	0.000	148274	0	<MDL	N.D. #
9)	A Endosulfan I	5.932	0.000	42554	0	<MDL	N.D. #
11)	B cis-Chlor...	5.932f	0.000	42554	0	<MDL	N.D. #
13)	MA Dieldrin	6.234	0.000	85312	0	<MDL	N.D. #
20)	A Methoxychlor	7.416f	0.000	5156545	0	8.217	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 17:47
Operator : AR\AJ
Sample : PB163566BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:15:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

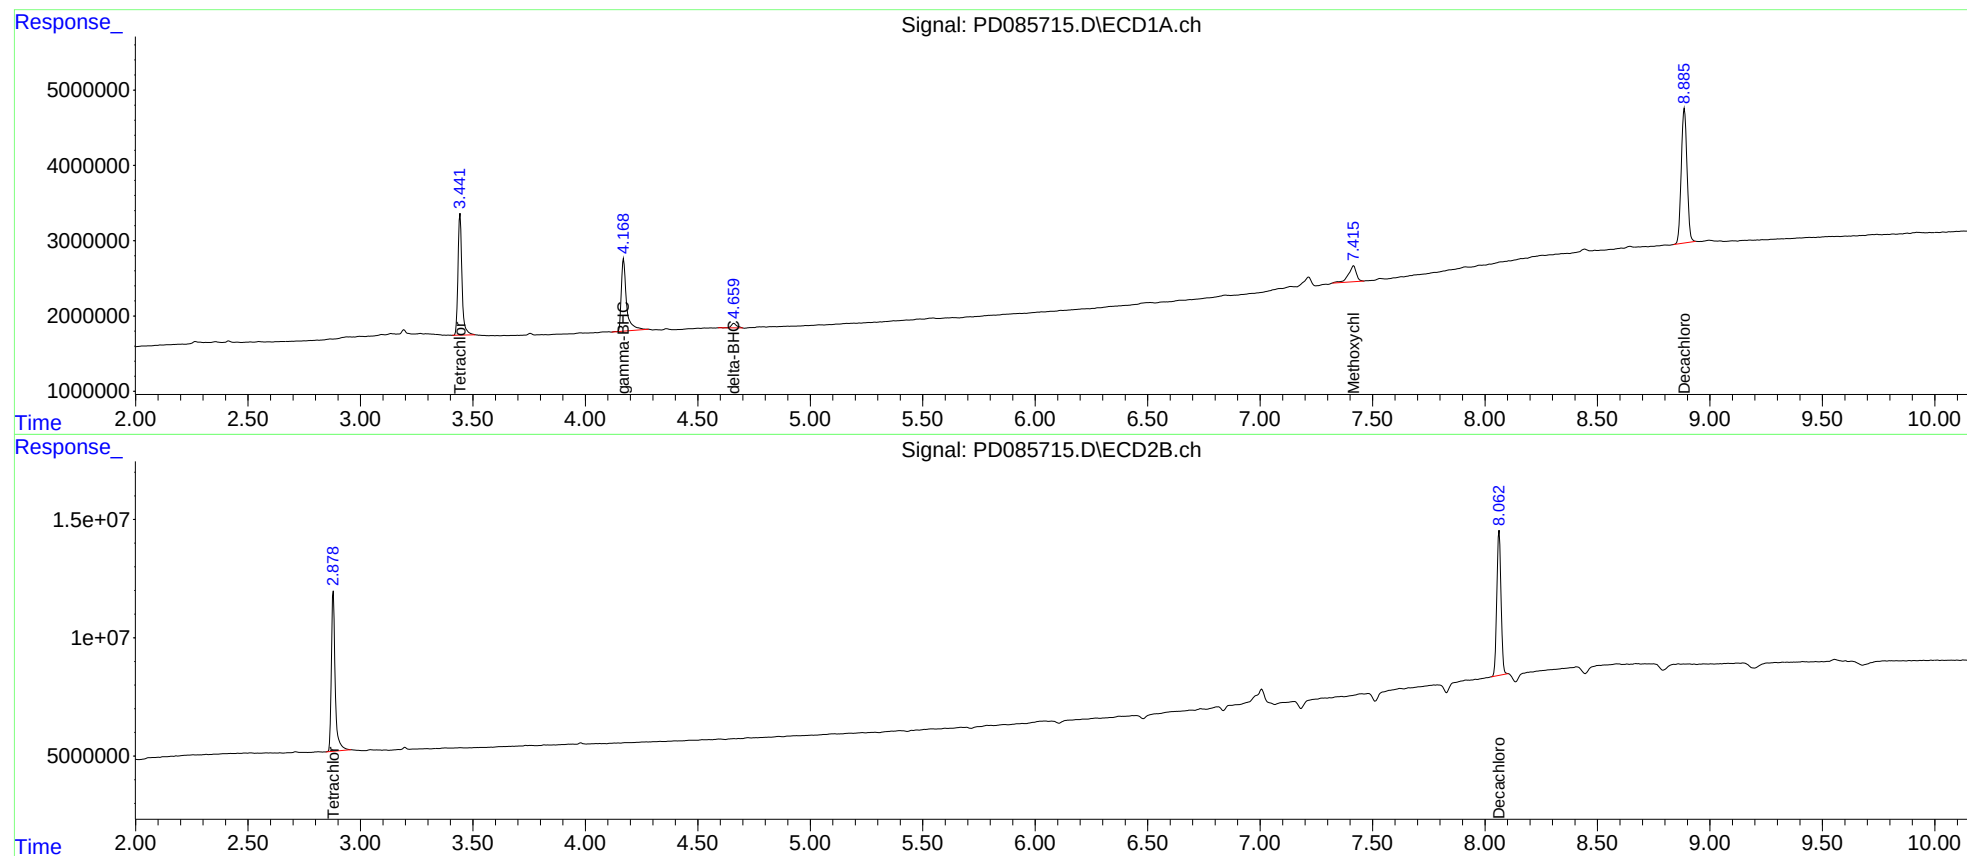

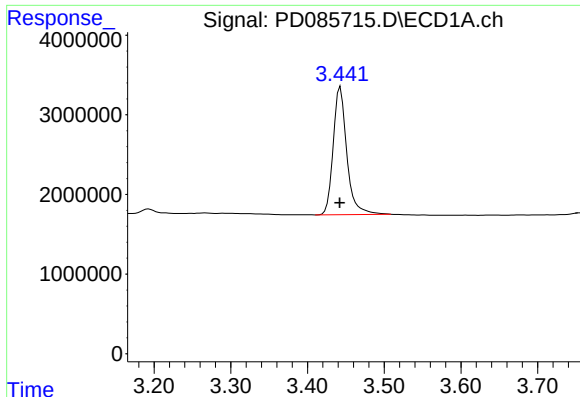


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 19818517
Conc: 18.92 ng/ml

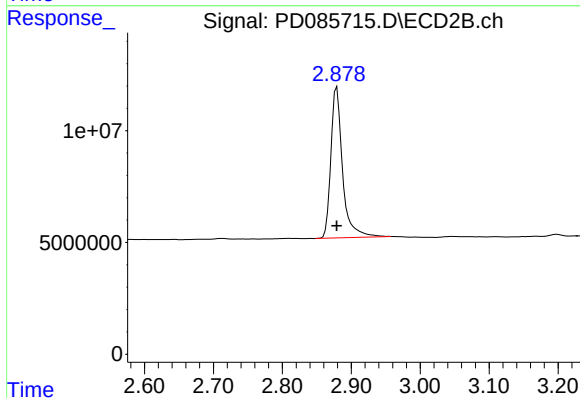


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 79416445
Conc: 18.76 ng/ml

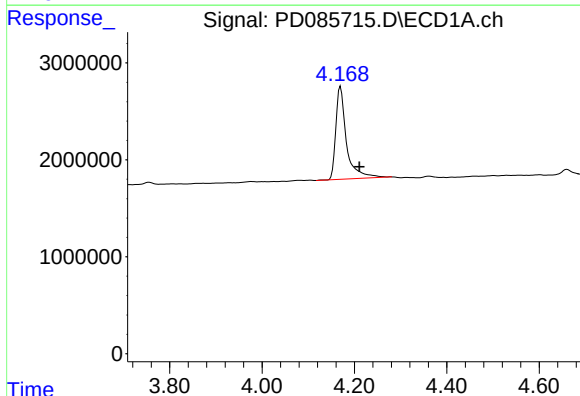


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: -0.041 min
Response: 15317116
Conc: 8.09 ng/ml

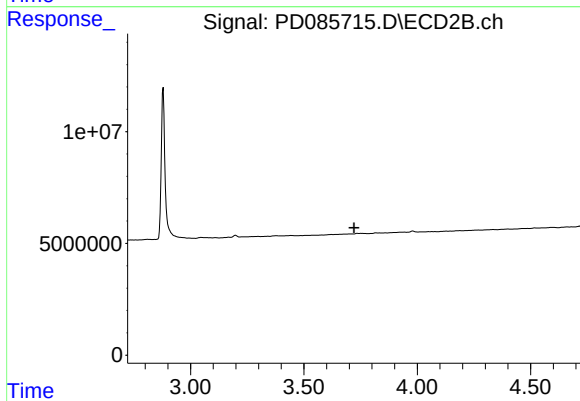


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.721 min
Response: 0
Conc: N.D.

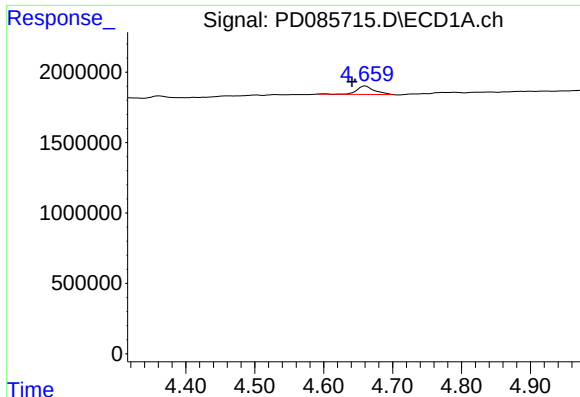


#7 delta-BHC

R.T.: 4.660 min
Delta R.T.: 0.019 min
Response: 1021191
Conc: 0.58 ng/ml

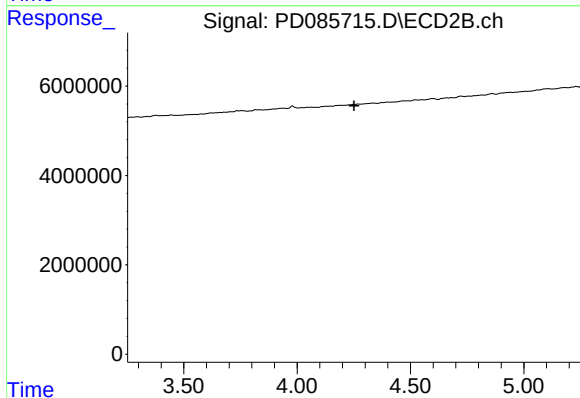


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.251 min
Response: 0
Conc: N.D.

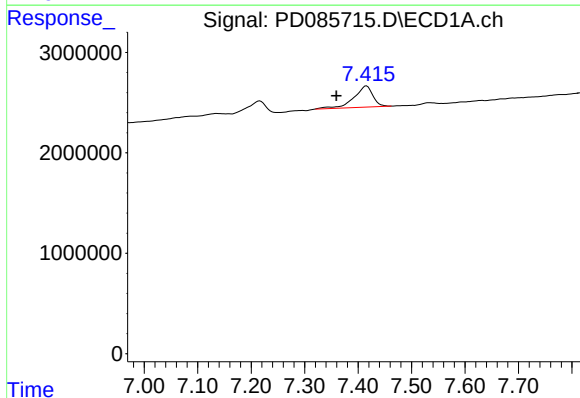


#20 Methoxychlor

R.T.: 7.416 min
Delta R.T.: 0.056 min
Response: 5156545
Conc: 8.22 ng/ml

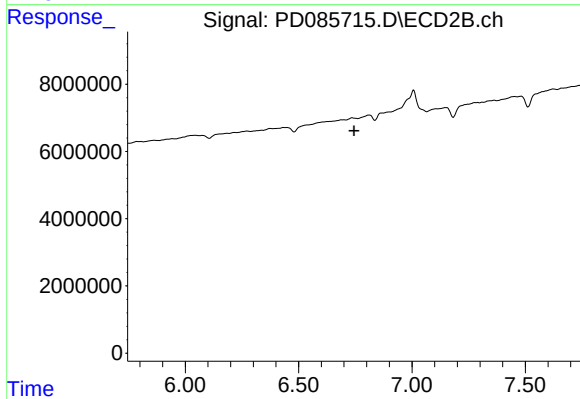


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.745 min
Response: 0
Conc: N.D.

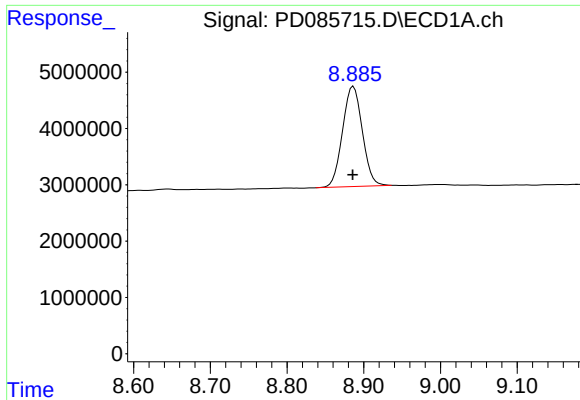

#27 Decachlorobiphenyl

R.T.: 8.886 min
Delta R.T.: 0.000 min
Response: 32088293
Conc: 21.77 ng/ml

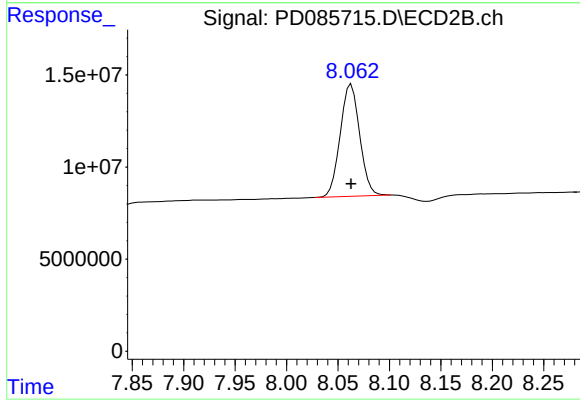

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 80223164
Conc: 20.75 ng/ml