

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 18:14
 Operator : AR\AJ
 Sample : PB163609BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:16:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.879	20206712	80823828	19.288	19.089
27)	SA Decachlor...	8.886	8.063	31742713	79677942	21.533	20.607
Target Compounds							
2)	A alpha-BHC	3.879	0.000	11837	0	<MDL	N.D. #
3)	MA gamma-BHC...	4.170f	0.000	11404385	0	6.024	N.D. #
4)	MA Heptachlor	4.788	0.000	63708	0	<MDL	N.D. #
7)	B delta-BHC	4.659	0.000	1061568	0	0.600	N.D. #
8)	B Heptachlo...	5.550	0.000	136180	0	<MDL	N.D. #
9)	A Endosulfan I	5.928	0.000	29166	0	<MDL	N.D. #
11)	B cis-Chlor...	5.928	0.000	29166	0	<MDL	N.D. #
13)	MA Dieldrin	6.227	0.000	91962	0	<MDL	N.D. #
16)	A 4,4'-DDD	6.568	0.000	31588	0	<MDL	N.D. #
18)	B Endrin al...	6.782	0.000	10805	0	<MDL	N.D. #
20)	A Methoxychlor	7.342	0.000	241385	0	0.385	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 18:14
Operator : AR\AJ
Sample : PB163609BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:16:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

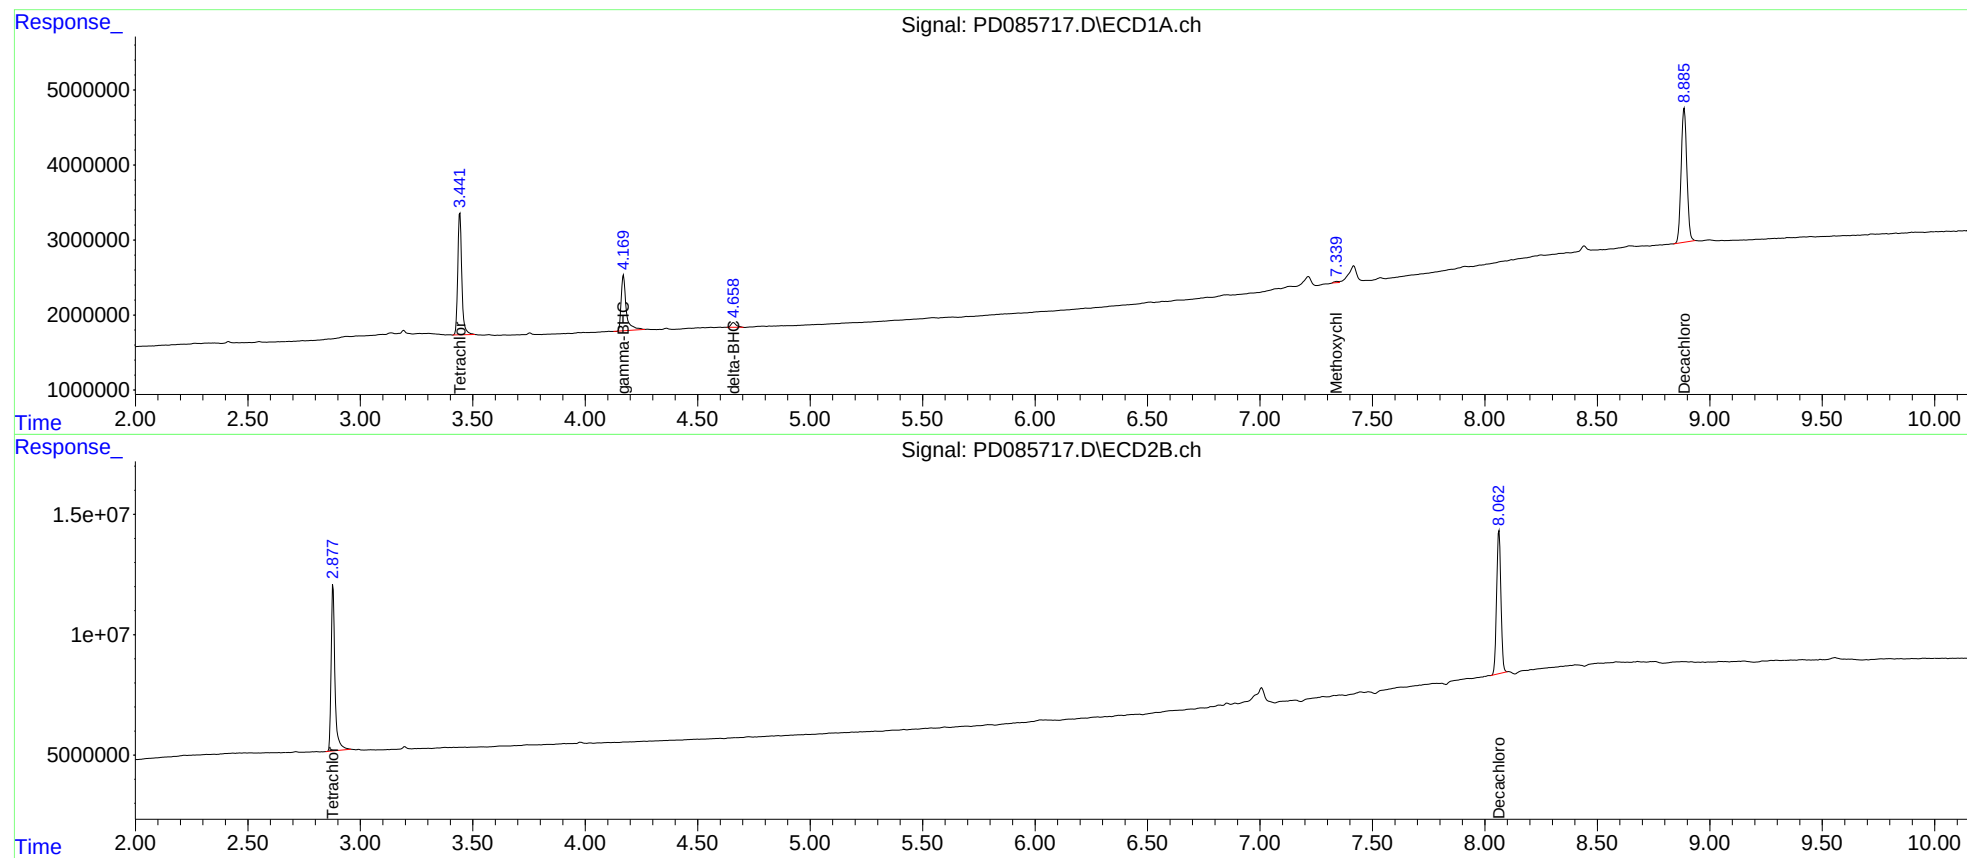

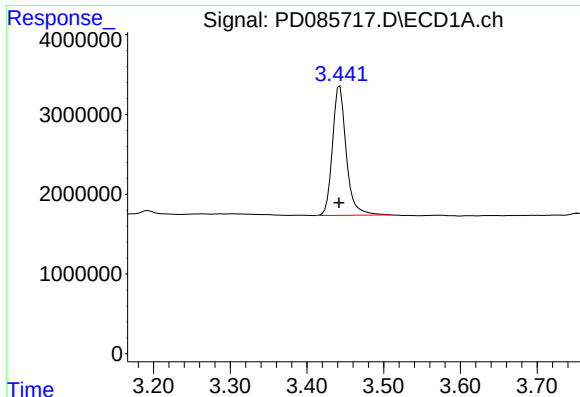


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 20206712
Conc: 19.29 ng/ml

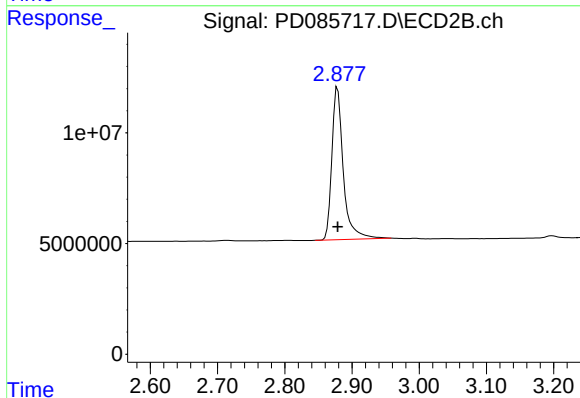


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 80823828
Conc: 19.09 ng/ml

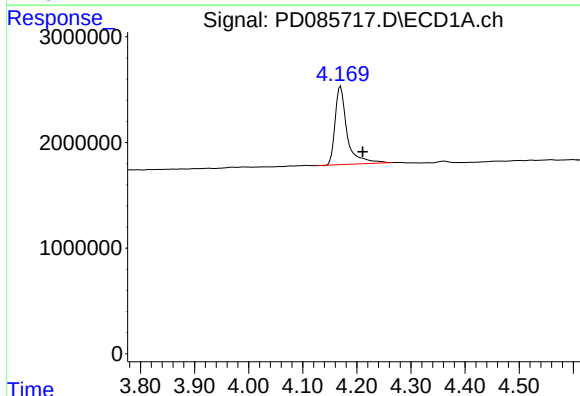


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: -0.041 min
Response: 11404385
Conc: 6.02 ng/ml

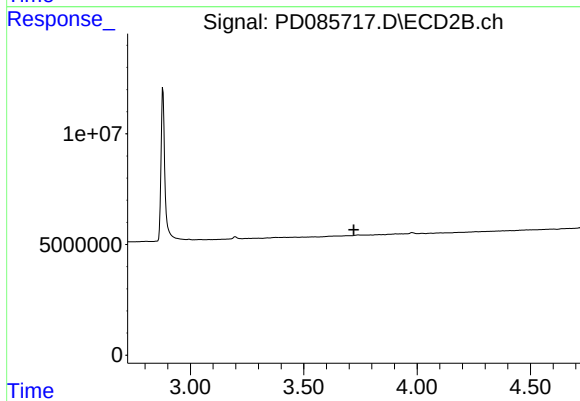


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.721 min
Response: 0
Conc: N.D.

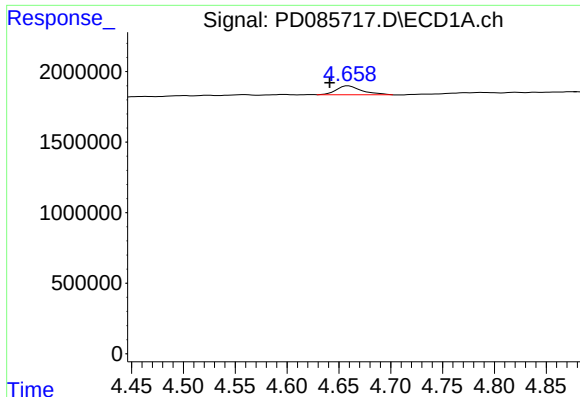


#7 delta-BHC

R.T.: 4.659 min
Delta R.T.: 0.018 min
Response: 1061568
Conc: 0.60 ng/ml

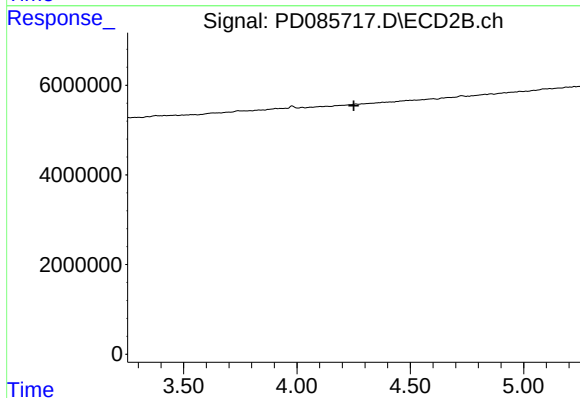


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.251 min
Response: 0
Conc: N.D.

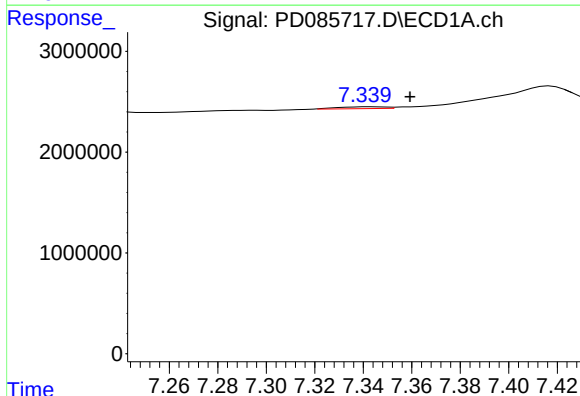


#20 Methoxychlor

R.T.: 7.342 min
Delta R.T.: -0.017 min
Response: 241385
Conc: 0.38 ng/ml

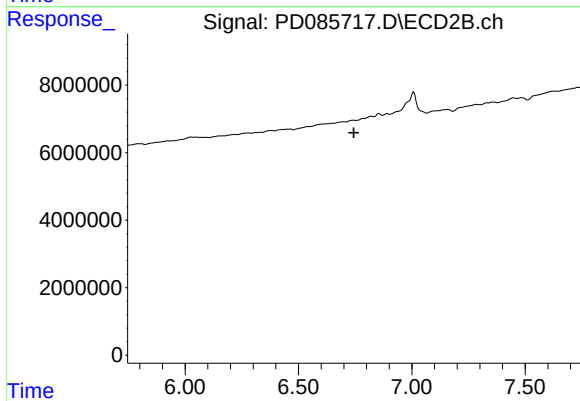


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.745 min
Response: 0
Conc: N.D.

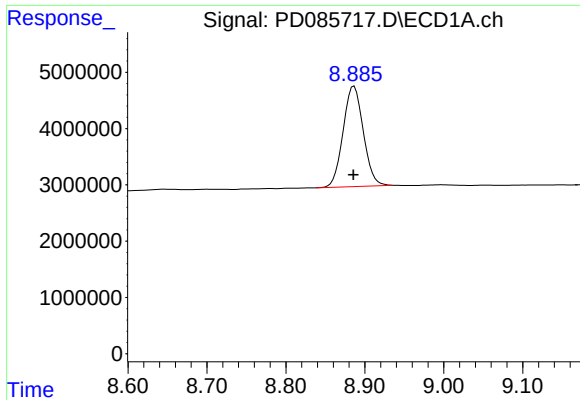

#27 Decachlorobiphenyl

R.T.: 8.886 min
Delta R.T.: 0.000 min
Response: 31742713
Conc: 21.53 ng/ml

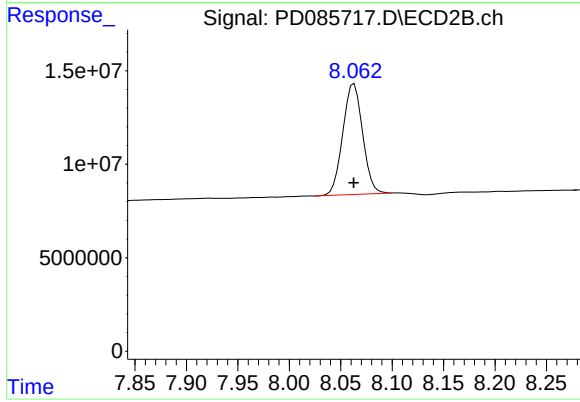

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 79677942
Conc: 20.61 ng/ml