

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 18:41
 Operator : AR\AJ
 Sample : PB163706BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:16:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.879	19802895	79164631	18.902	18.697
27)	SA Decachlor...	8.887	8.063	31404431	78211931	21.304	20.228
Target Compounds							
2)	A alpha-BHC	3.890	0.000	5376	0	<MDL	N.D. #
3)	MA gamma-BHC...	4.170f	0.000	10152986	0	5.363	N.D. #
4)	MA Heptachlor	4.787	0.000	56210	0	<MDL	N.D. #
5)	MB Aldrin	5.159	0.000	60709	0	<MDL	N.D. #
7)	B delta-BHC	4.659	0.000	861880	0	0.487	N.D. #
8)	B Heptachlo...	5.548	0.000	165600	0	0.106	N.D. #
9)	A Endosulfan I	5.938	0.000	28905	0	<MDL	N.D. #
11)	B cis-Chlor...	5.938f	0.000	28905	0	<MDL	N.D. #
16)	A 4,4'-DDD	6.576	0.000	59532	0	<MDL	N.D. #
20)	A Methoxychlor	7.417f	0.000	4701783	0	7.493	N.D. #
23)	Toxaphene-2	6.356f	0.000	97594	0	6.551	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 18:41
Operator : AR\AJ
Sample : PB163706BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:16:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

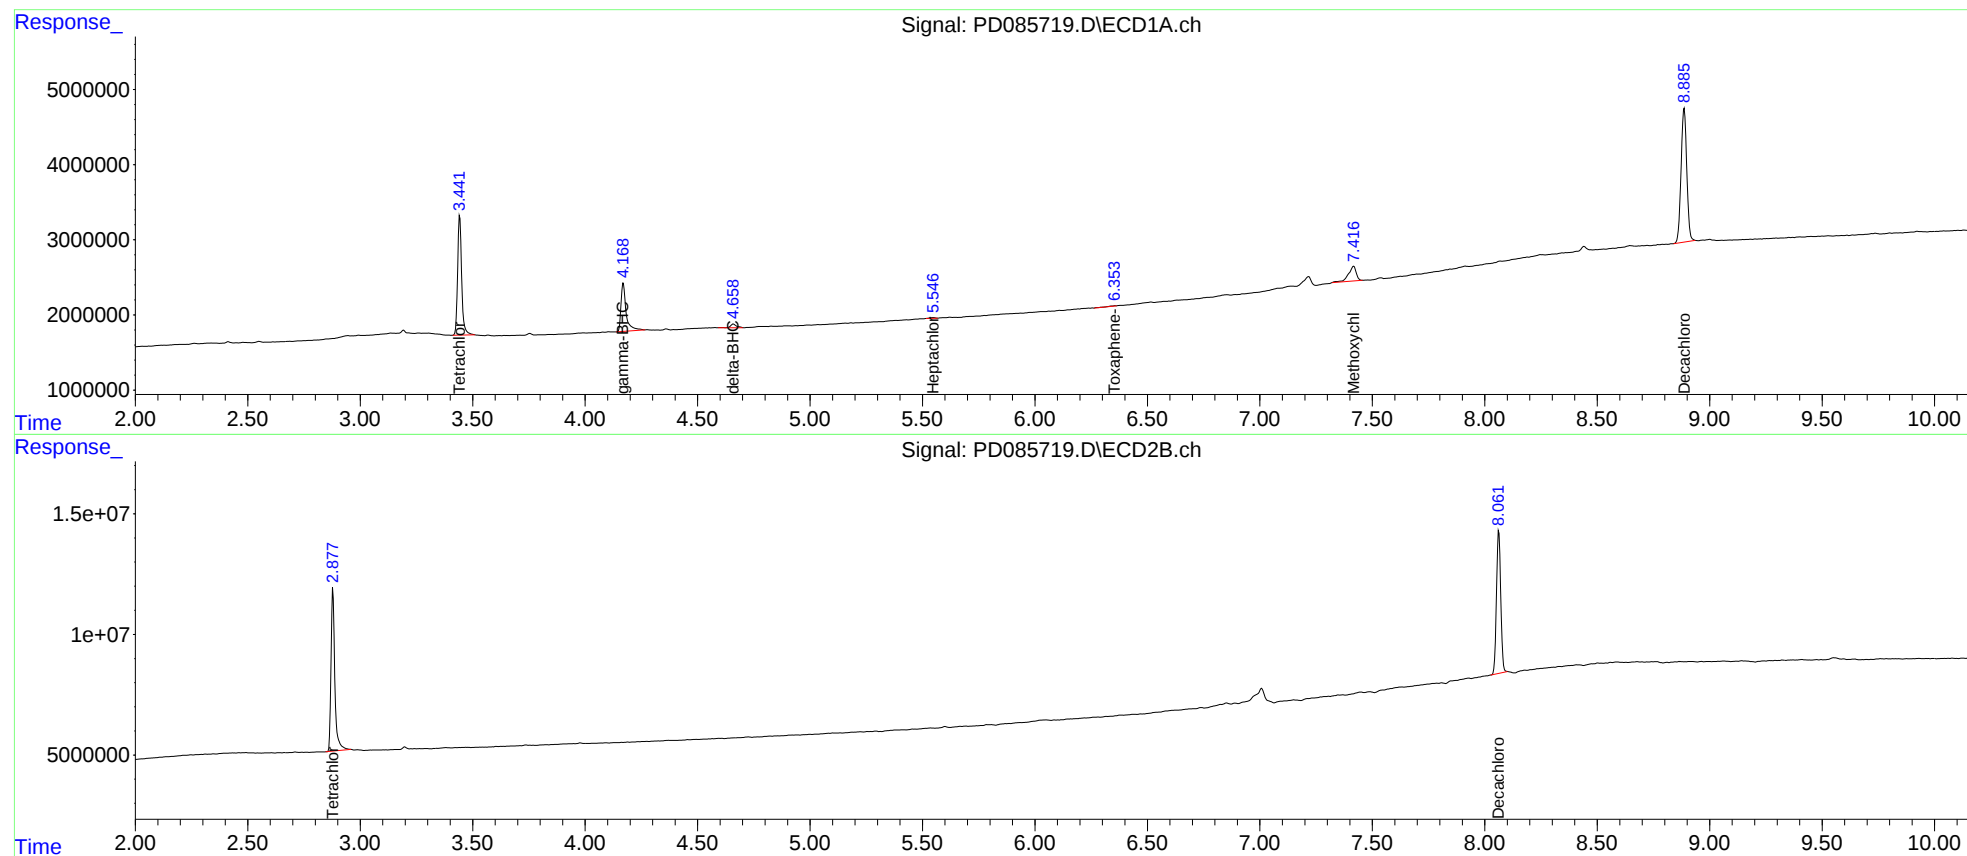

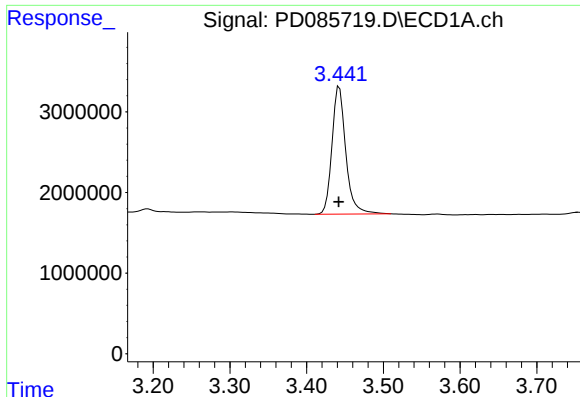


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 19802895
Conc: 18.90 ng/ml

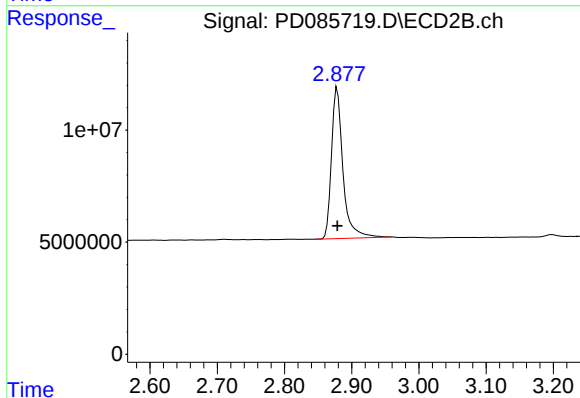


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 79164631
Conc: 18.70 ng/ml

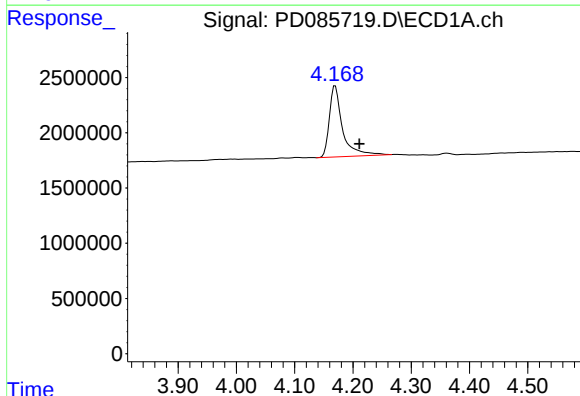


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: -0.041 min
Response: 10152986
Conc: 5.36 ng/ml

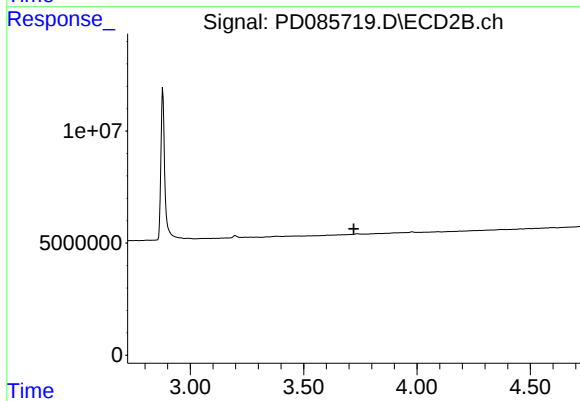


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.721 min
Response: 0
Conc: N.D.

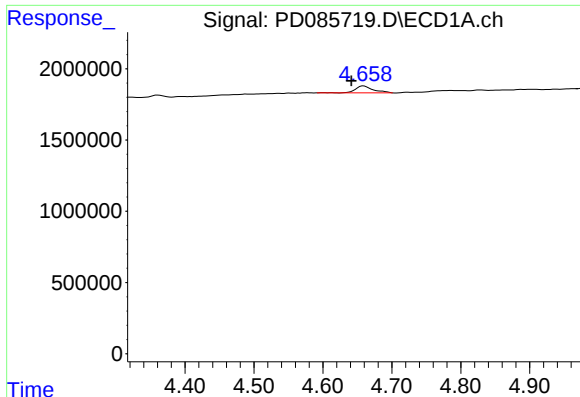


#7 delta-BHC

R.T.: 4.659 min
Delta R.T.: 0.018 min
Response: 861880
Conc: 0.49 ng/ml

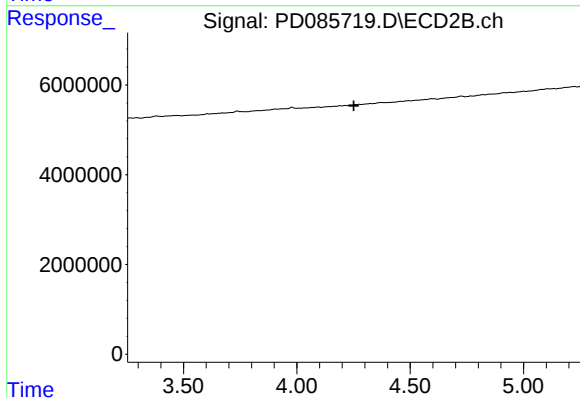


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.251 min
Response: 0
Conc: N.D.

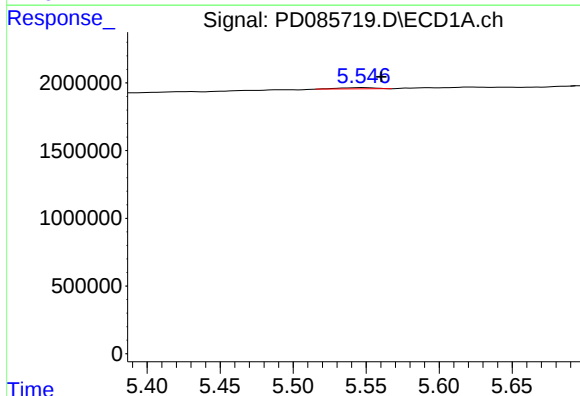


#8 Heptachlor epoxide

R.T.: 5.548 min
Delta R.T.: -0.013 min
Response: 165600
Conc: 0.11 ng/ml

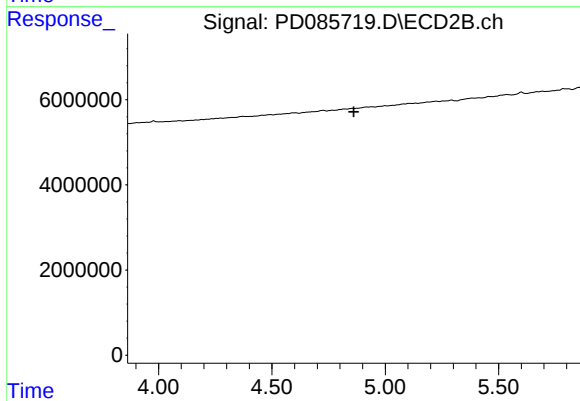


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.861 min
Response: 0
Conc: N.D.

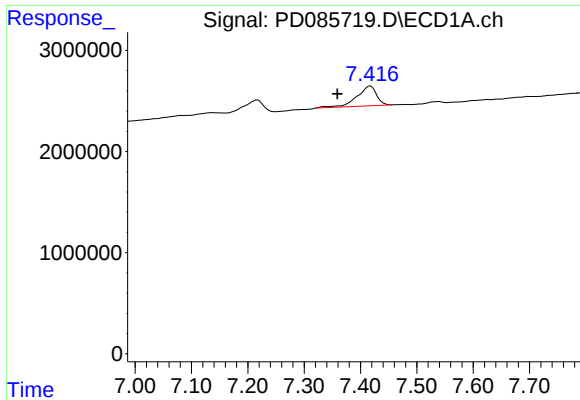


#20 Methoxychlor

R.T.: 7.417 min
Delta R.T.: 0.058 min
Response: 4701783
Conc: 7.49 ng/ml

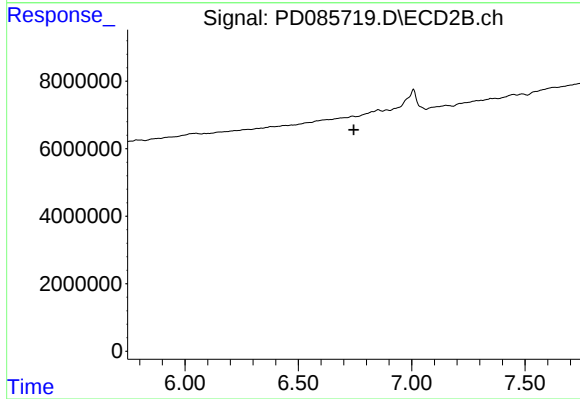


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.745 min
Response: 0
Conc: N.D.

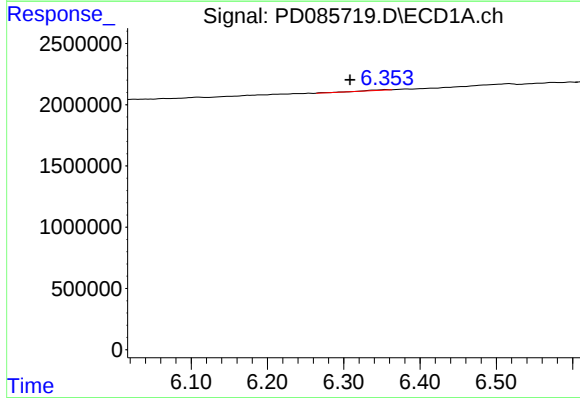


#23 Toxaphene-2

R.T.: 6.356 min
Delta R.T.: 0.048 min
Response: 97594
Conc: 6.55 ng/ml

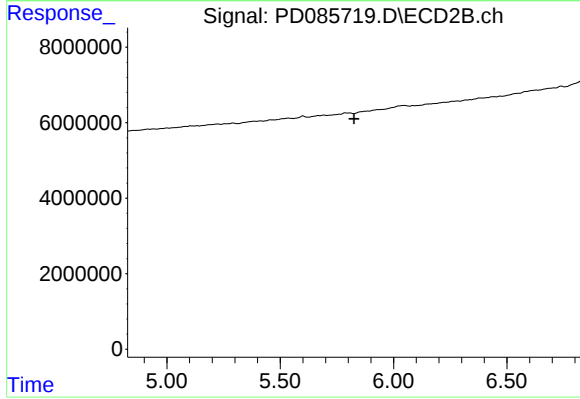


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.826 min
Response: 0
Conc: N.D.

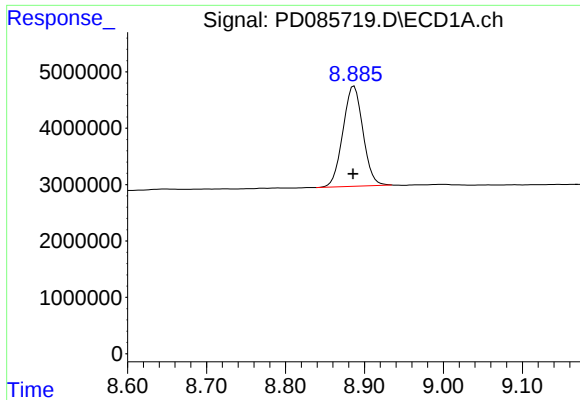

#27 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: 0.001 min
Response: 31404431
Conc: 21.30 ng/ml

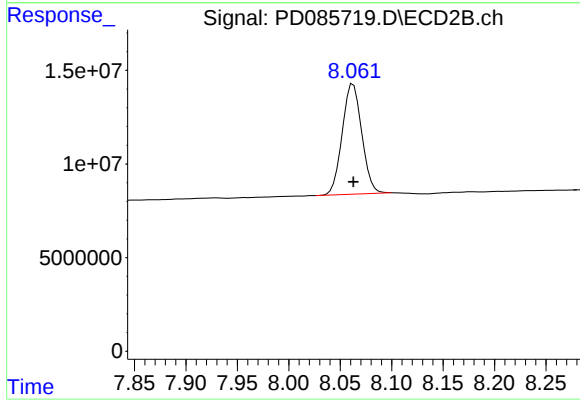

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 78211931
Conc: 20.23 ng/ml