


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 11:09
Operator : AR\AJ
Sample : RESC046
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 15:22:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

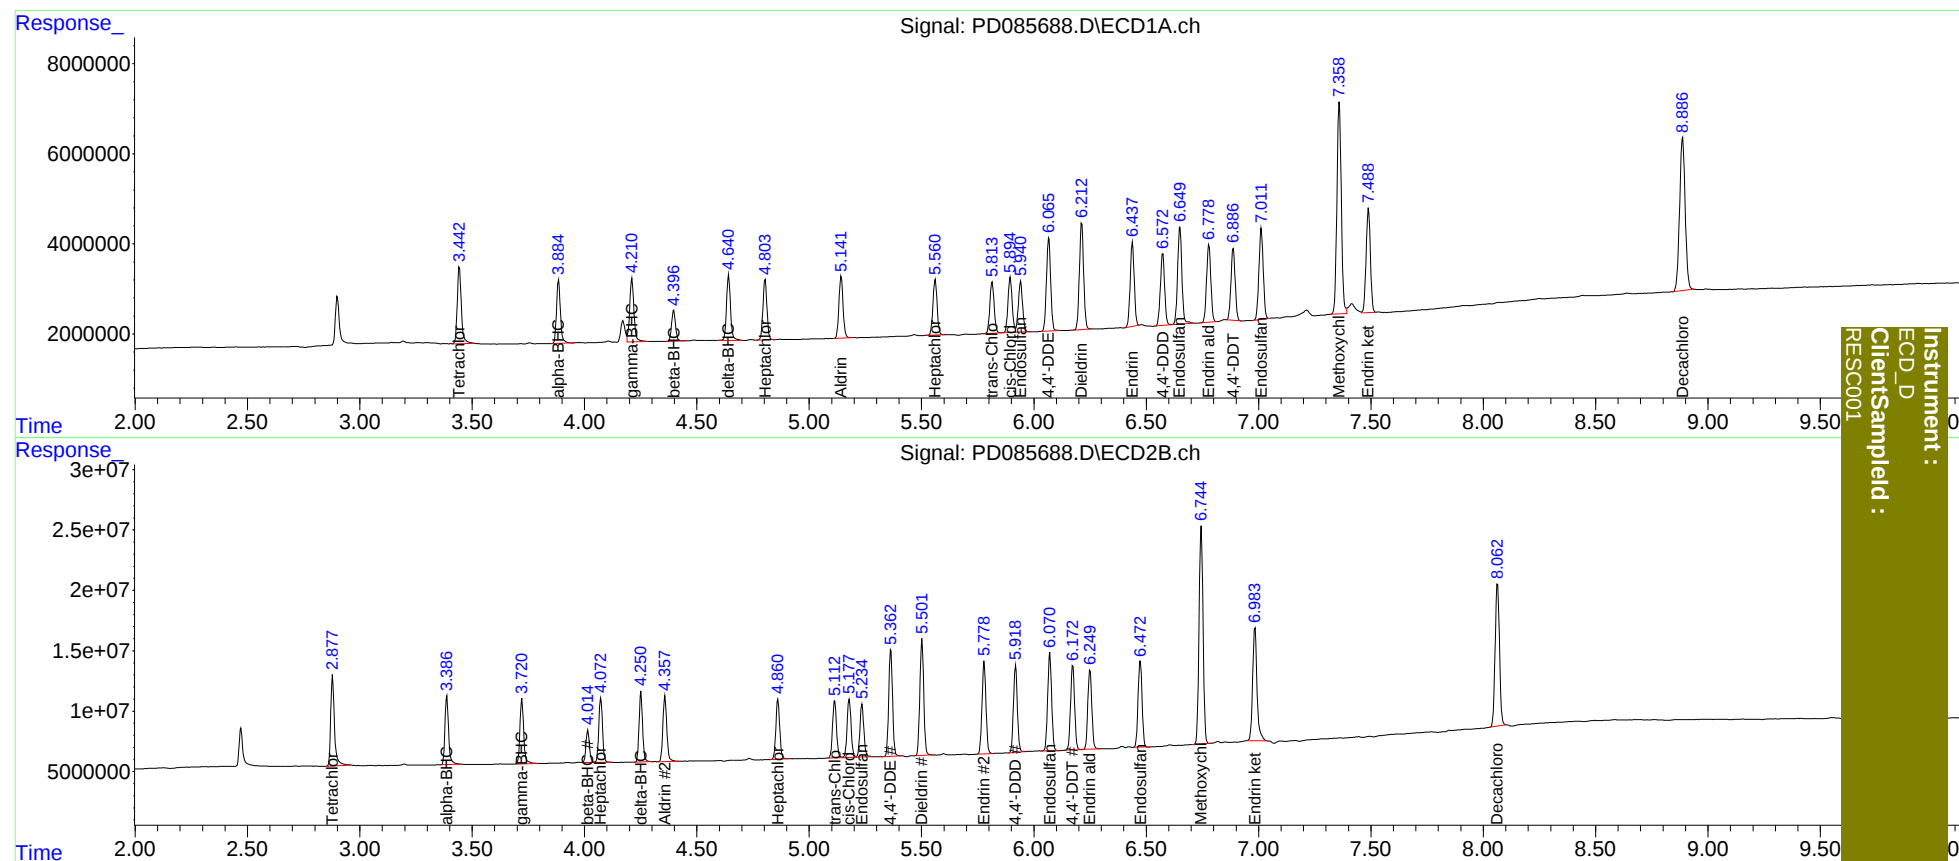

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 11:09
 Operator : AR\AJ
 Sample : RESC046
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 15:22:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.879	21244630	87159388	20.279	20.585
2)	SA Decachlor...	8.887	8.064	58776675	157.8E6	39.872	40.820
Target Compounds							
2)	A alpha-BHC	3.885	3.388	16996872	64805634	9.339	10.034
3)	MA gamma-BHC...	4.212	3.722	18393167	62433671	9.716	10.136
4)	MA Heptachlor	4.804	4.073	16668572	60550037	9.749	10.128
5)	MB Aldrin	5.143	4.358	17547201	65512006	10.434	11.007
6)	B beta-BHC	4.397	4.015	8383618	28982716	10.704	10.838
7)	B delta-BHC	4.642	4.252	17971758	63619510	10.154	10.671
8)	B Heptachlo...	5.561	4.861	16077912	59065436	10.282	10.770
9)	A Endosulfan I	5.941	5.235	14797437	52590119	9.898	10.266
10)	B trans-Chl...	5.814	5.114	15260692	57991147	10.225	10.713
11)	B cis-Chlor...	5.895	5.179	15854362	59112844	10.167	10.696
12)	B 4,4'-DDE	6.067	5.363	26967188	105.8E6	19.874	21.264
13)	MA Dieldrin	6.213	5.502	30999651	114.8E6	18.989	20.326
14)	MA Endrin	6.439	5.779	23414427	93212539	19.500	20.770
15)	B Endosulfa...	6.650	6.071	28646565	100.2E6	20.925	21.814
16)	A 4,4'-DDD	6.574	5.919	20950149	86479202	19.017	20.341
17)	MA 4,4'-DDT	6.887	6.173	20604622	87744830	18.539	20.075
18)	B Endrin al...	6.779	6.250	22822294	80763056	21.916	23.065
19)	B Endosulfa...	7.012	6.474	26954334	89064500	20.860	21.252
20)	A Methoxychlor	7.359	6.745	64047249	223.5E6	102.063	106.037
21)	B Endrin ke...	7.489	6.984	30420389	125.7E6	21.733	23.566

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.