

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 20:29
 Operator : AR\AJ
 Sample : P4010-03MS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW6MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/29/2024
 Supervised By :Ankita Jodhani 09/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:19:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.443	2.879	3890014	14741538	3.713	3.482
27) SA Decachlor...	8.884	8.063	5719198	11078726	3.880	2.865 #
Target Compounds						
2) A alpha-BHC	3.885	3.388	52602485	175.7E6	28.903	27.207
3) MA gamma-BHC...	4.211	3.722	59851937	169.9E6	31.615	27.586
4) MA Heptachlor	4.804	4.072	51041836	228.1E6	29.854	38.156 #
5) MB Aldrin	5.143	4.358	50729670	169.6E6	30.164	28.498
6) B beta-BHC	4.397	4.015	20531635	68257966	26.215	25.524
7) B delta-BHC	4.641	4.251	57687685	167.7E6	32.592m	28.127
8) B Heptachlo...	5.561	4.860	43934388	155.2E6	28.096	28.293
9) A Endosulfan I	5.941	5.235	44189923	144.9E6	29.558	28.293
10) B trans-Chl...	5.815	5.113	46493182	168.1E6	31.153	31.044
11) B cis-Chlor...	5.895	5.178	49888157	168.4E6	31.991	30.464
12) B 4,4'-DDE	6.066	5.363	84669382	279.9E6	62.399	56.255
13) MA Dieldrin	6.213	5.502	96257767	313.0E6	58.962	55.393
14) MA Endrin	6.437	5.777	82116670	280.4E6	68.389m	62.489m
15) B Endosulfa...	6.651	6.071	79289677	290.2E6	57.916	63.185
16) A 4,4'-DDD	6.573	5.919	67206695	227.2E6	61.004	53.441
17) MA 4,4'-DDT	6.886	6.173	69417179	249.1E6	62.459m	56.997
18) B Endrin al...	6.779	6.249	63322772	199.4E6	60.808	56.937
19) B Endosulfa...	7.013	6.473	78510241	291.1E6	60.760	69.459m
20) A Methoxychlor	7.360	6.745	201.3E6	567.3E6	320.738	269.147
21) B Endrin ke...	7.489	6.984	89034062	300.4E6	63.608	56.325

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 20:29
Operator : AR\AJ
Sample : P4010-03MS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:19:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

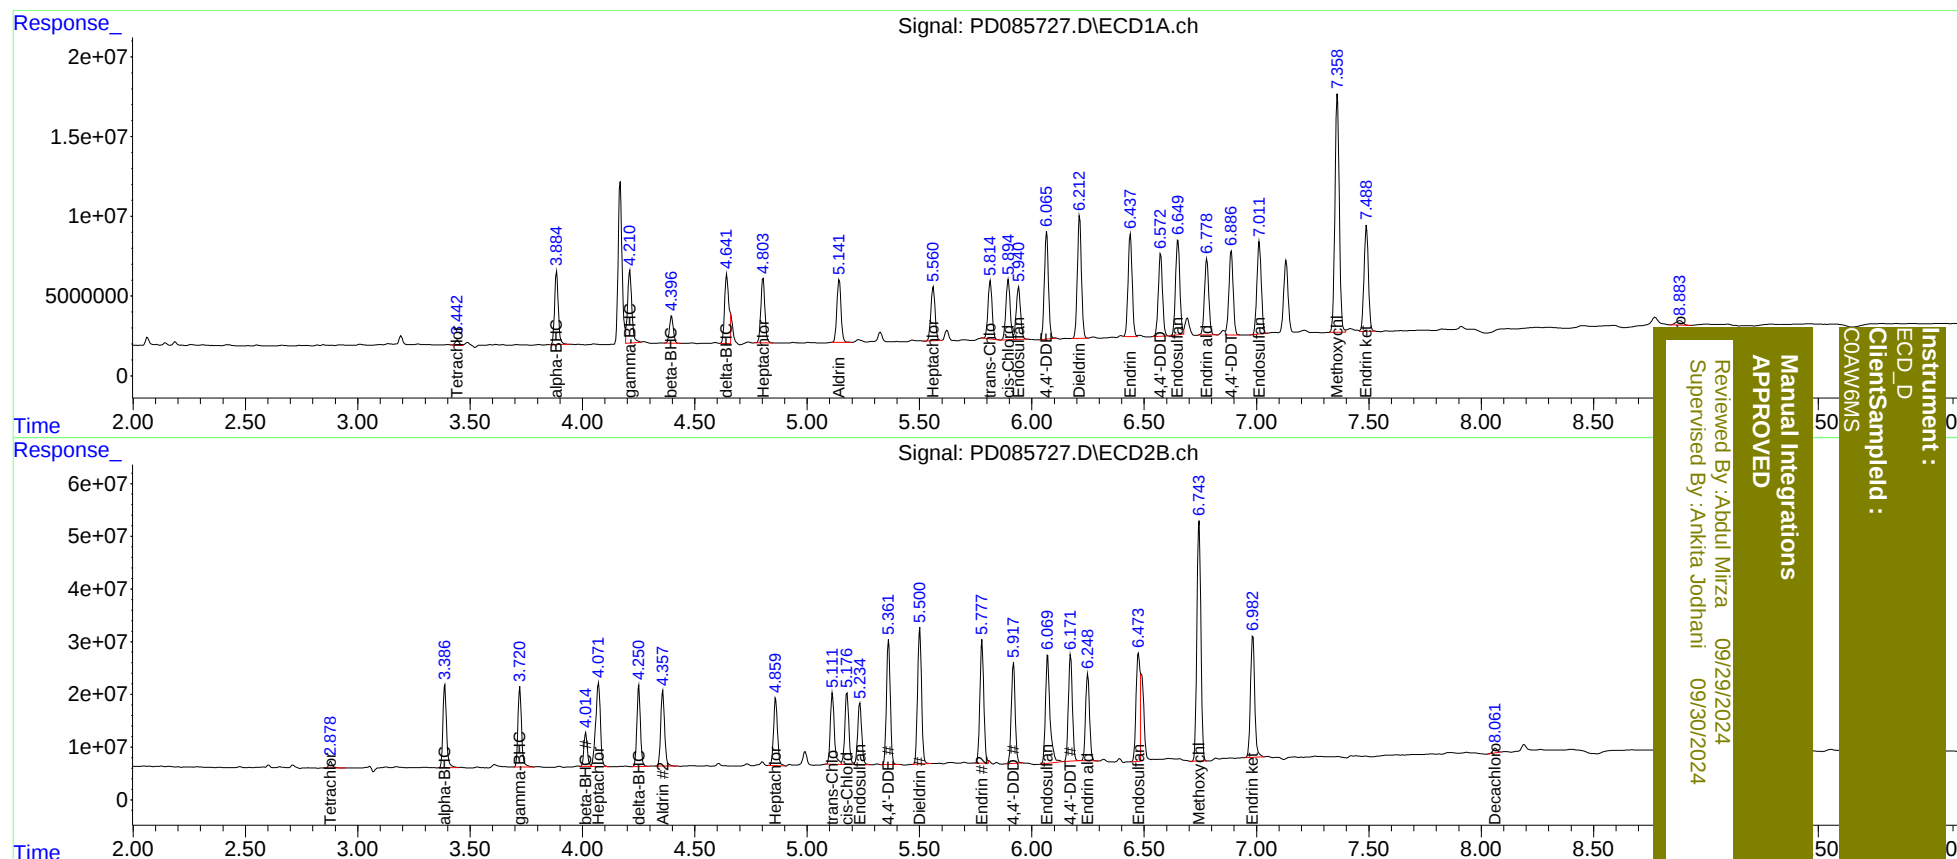

Instrument :
ECD_D
Client Sampled :
COAW6MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/29/2024
Supervised By: Ankita Jodhani 09/30/2024