

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 20:42
 Operator : AR\AJ
 Sample : P4010-04MSD
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/29/2024
 Supervised By :Ankita Jodhani 09/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:19:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.441	2.878	3736302	15151552	3.566m	3.578m
2) SA Decachlor...	8.885	8.063	5632751	11106512	3.821	2.872
Target Compounds						
2) A alpha-BHC	3.885	3.388	52844285	178.1E6	29.036	27.582
3) MA gamma-BHC...	4.211	3.722	59986312	171.8E6	31.686	27.884
4) MA Heptachlor	4.804	4.072	51398467	229.8E6	30.062	38.432 #
5) MB Aldrin	5.143	4.358	50738633	170.5E6	30.170	28.655
6) B beta-BHC	4.397	4.015	20824909	69327130	26.590	25.924
7) B delta-BHC	4.641	4.252	51634363	168.2E6	29.172m	28.207
8) B Heptachlo...	5.559	4.861	45808792	156.3E6	29.294m	28.500
9) A Endosulfan I	5.942	5.235	44209776	145.5E6	29.571	28.398
10) B trans-Chl...	5.815	5.113	46542944	168.7E6	31.186	31.169
11) B cis-Chlor...	5.895	5.178	50148151	169.1E6	32.158	30.593
12) B 4,4'-DDE	6.066	5.362	84876749	282.7E6	62.552	56.823
13) MA Dieldrin	6.213	5.501	96071382	315.7E6	58.848	55.871
14) MA Endrin	6.437	5.777	81608057	283.8E6	67.965m	63.230m
15) B Endosulfa...	6.651	6.071	78251509	294.1E6	57.158	64.032
16) A 4,4'-DDD	6.573	5.918	67295333	229.3E6	61.084	53.927
17) MA 4,4'-DDT	6.887	6.173	64348741	250.2E6	57.898	57.249
18) B Endrin al...	6.779	6.249	63446787	200.4E6	60.927	57.235
19) B Endosulfa...	7.013	6.473	79335280	296.7E6	61.398	70.792m
20) A Methoxychlor	7.360	6.745	201.2E6	580.2E6	320.584	275.244
21) B Endrin ke...	7.489	6.984	86375891	301.2E6	61.709	56.465

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 20:42
Operator : AR\AJ
Sample : P4010-04MSD
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:19:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

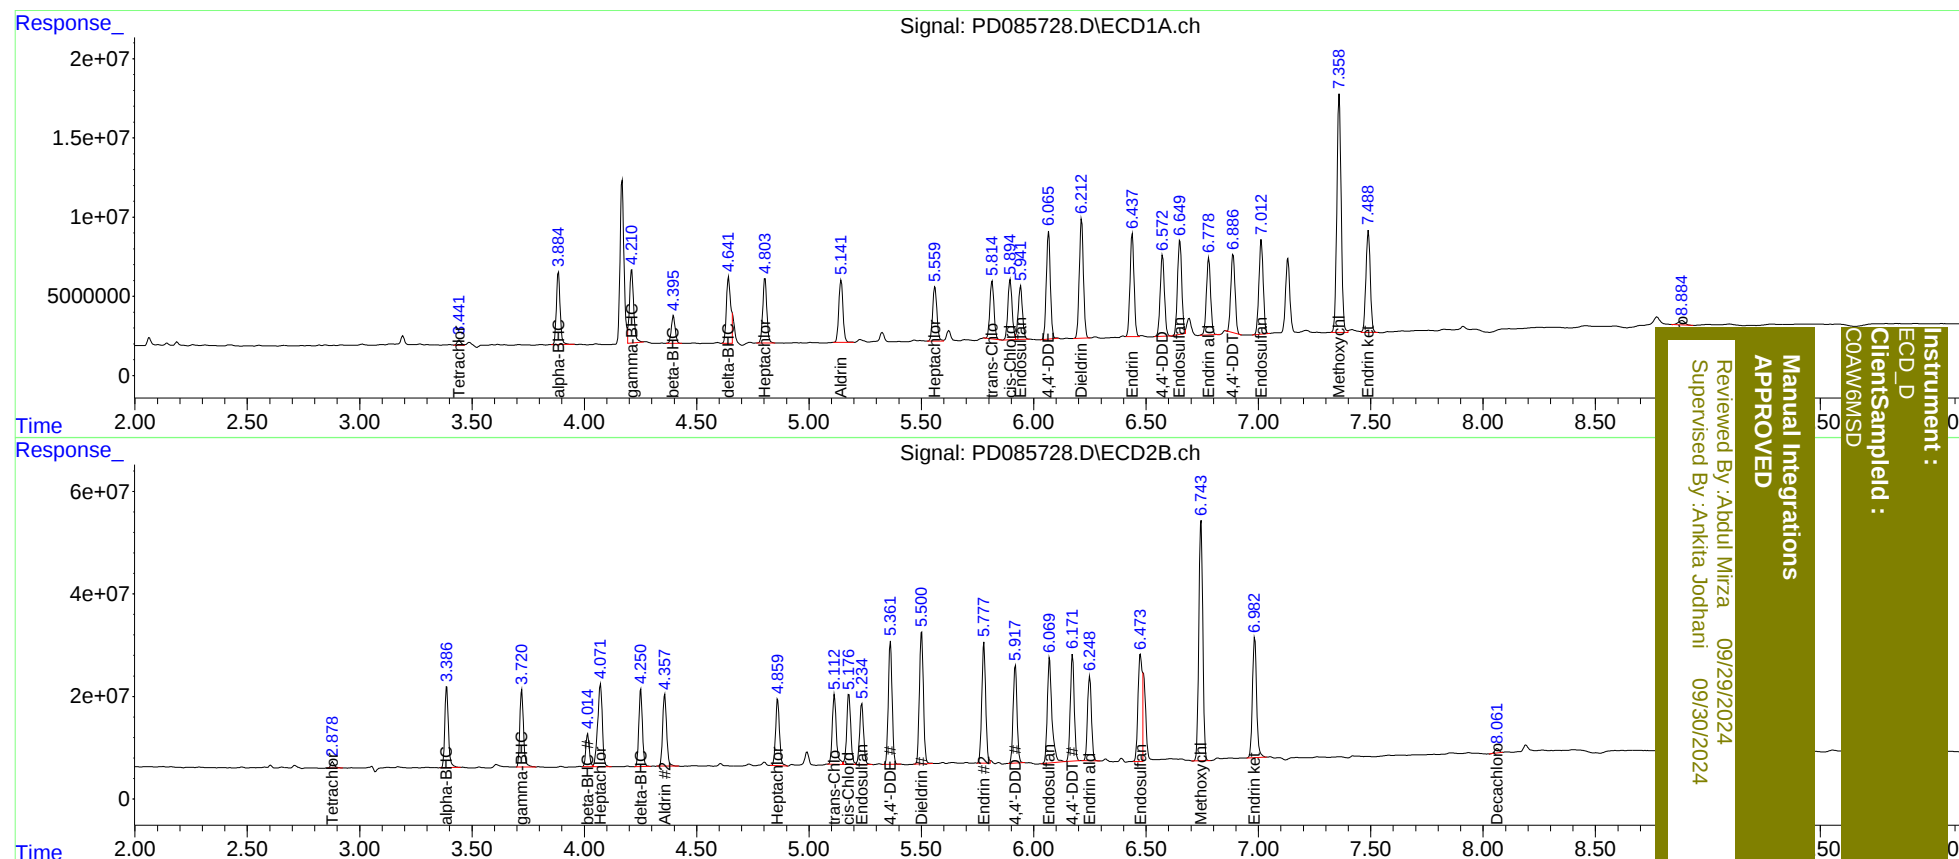

Instrument :
ECD_D
Client Sampled :
COAW6MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/29/2024
Supervised By: Ankita Jodhani 09/30/2024