

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
 Data File : PD085739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 00:18
 Operator : AR\AJ
 Sample : P4017-08MS
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC70MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/29/2024
 Supervised By :Ankita Jodhani 09/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:24:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.429	2.889	29293400	419.2E6	27.961m	99.011m#
27) SA Decachlor...	8.883	8.062	27278558	55738040	18.505m	14.416m
Target Compounds						
2) A alpha-BHC	3.885	3.387	1346.6E6	2860.3E6	739.923	442.855 #
3) MA gamma-BHC...	4.149f	3.718	99369.4E6	1601.4E6	52488.987m	259.987m#
4) MA Heptachlor	4.803	4.056	134.4E6	258.3E6	78.611m	43.209m#
5) MB Aldrin	5.144	4.348	93169524	287.5E6	55.399m	48.301m
6) B beta-BHC	4.394	4.011	167.7E6	234.0E6	214.065m	87.488m#
7) B delta-BHC	4.643	4.252	1938.3E6	3422.0E6	1095.124	573.968 #
8) B Heptachlo...	5.557	4.856	90254969	911.6E6	57.717	166.220m#
9) A Endosulfan I	5.944	5.236	94884738	158.5E6	63.467	30.934 #
10) B trans-Chl...	5.813	5.112	84772600	240.8E6	56.802	44.474m
11) B cis-Chlor...	5.893	5.180	100.6E6	271.8E6	64.510	49.175
12) B 4,4'-DDE	6.067	5.362	178.7E6	345.8E6	131.705	69.488 #
13) MA Dieldrin	6.212	5.500	261.1E6	352.3E6	159.965m	62.354m#
14) MA Endrin	6.437	5.778	129.6E6	470.5E6	107.928m	104.835m
15) B Endosulfa...	6.650	6.069	95805918	418.5E6	69.980m	91.115m#
16) A 4,4'-DDD	6.573	5.919	1162.8E6	2397.3E6	1055.521	563.877 #
17) MA 4,4'-DDT	6.888	6.172	157.4E6	523.2E6	141.582	119.702
18) B Endrin al...	6.777	6.248	111.8E6	218.8E6	107.317m	62.500m#
19) B Endosulfa...	7.012	6.474	125.8E6	268.6E6	97.325	64.091 #
20) A Methoxychlor	7.359	6.741	349.9E6	985.9E6	557.531	467.718m
21) B Endrin ke...	7.485	6.983	330.2E6	384.8E6	235.874m	72.141 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092724\
Data File : PD085739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 00:18
Operator : AR\AJ
Sample : P4017-08MS
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:24:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

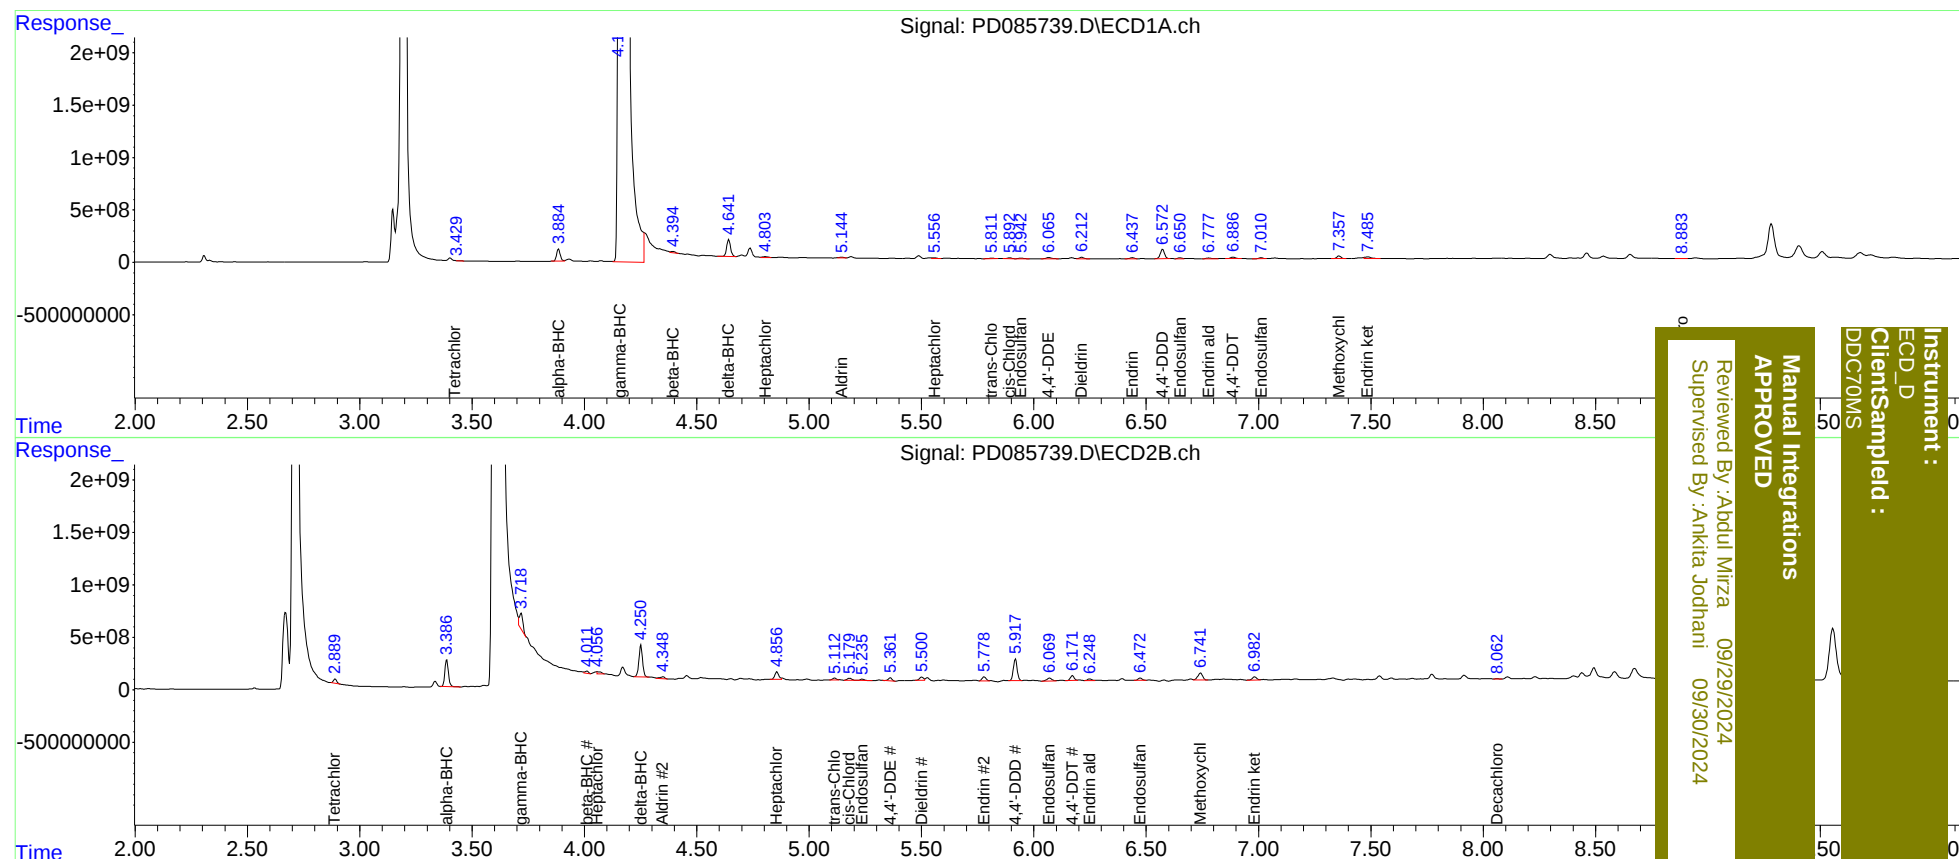

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/29/2024
Supervised By: Ankita Jodhani 09/30/2024

Instrument :
ECD_D
Client Sampled :
DDC70MS