

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
 Data File : PD059393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2020 12:42
 Operator : DD\AJ
 Sample : MDL-TOX-BL-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 13:13:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.512	4.025	26838783	37135571	21.396	22.069
27)	SA Decachlor...	8.323	9.111	35720076	49715373	42.329	43.672
Target Compounds							
2)	A alpha-BHC	3.974	0.000	430844	0	0.244	N.D. #
6)	B beta-BHC	4.462f	0.000	1415003	0	1.834	N.D. #
8)	B Heptachlo...	0.000	5.919	0	846588	N.D.	0.450
10)	B trans-Chl...	5.479	0.000	41773	0	<MDL	N.D. #
11)	B cis-Chlor...	5.479f	0.000	41773	0	<MDL	N.D. #
15)	B Endosulfa...	0.000	6.952	0	646669	N.D.	0.453
16)	A 4,4'-DDD	6.296f	6.823f	1061476	236237	1.022	0.175 #
19)	B Endosulfa...	6.782	0.000	192541	0	0.190	N.D. #
20)	A Methoxychlor	0.000	7.553f	0	207300	N.D.	0.334
24)	Toxaphene-3	6.296	0.000	1061476	0	129.057	N.D. #
26)	Toxaphene-5	7.106	0.000	2669039	0	156.626	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
Data File : PD059393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2020 12:42
Operator : DD\AJ
Sample : MDL-TOX-BL-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 13:13:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

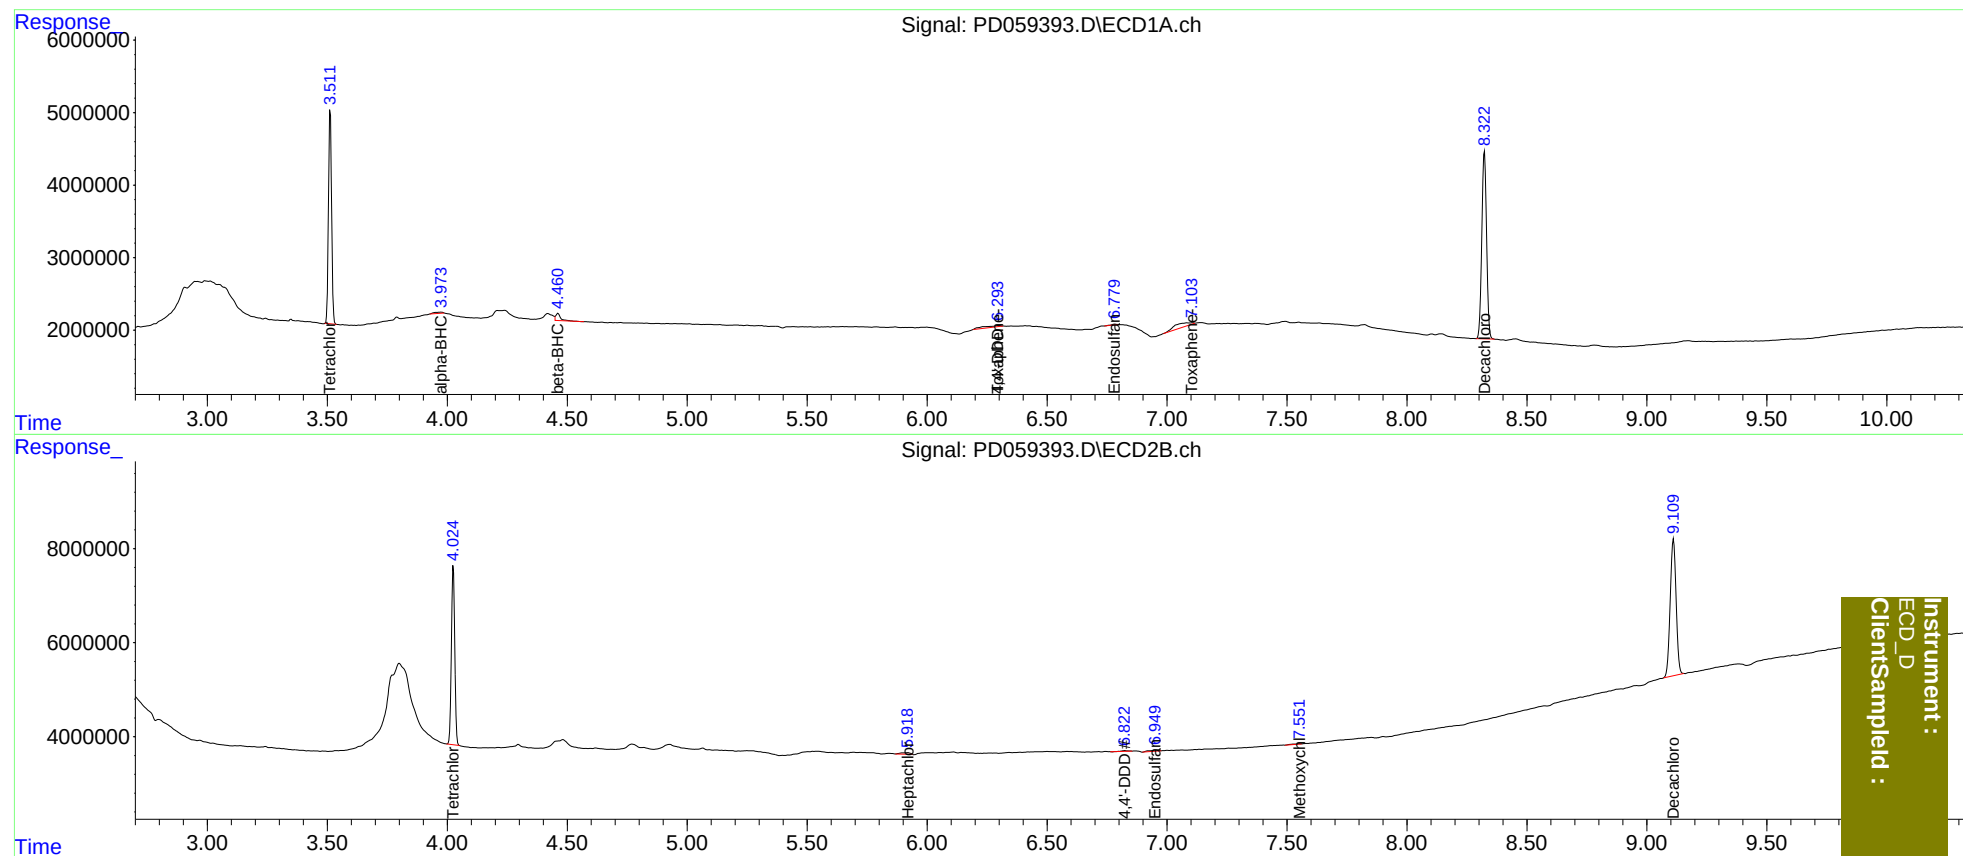


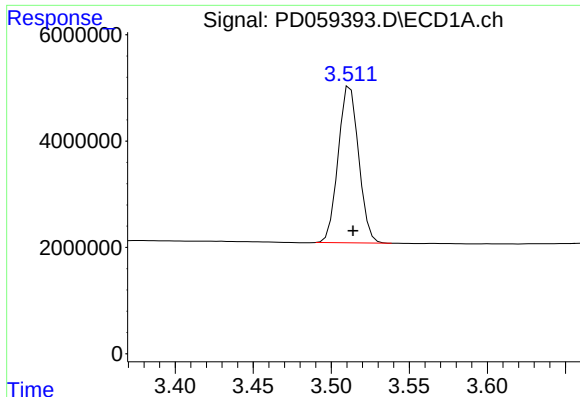

#1 Tetrachloro-m-xylene


R.T.: 3.512 min
Delta R.T.: -0.002 min
Response: 26838783
Conc: 21.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

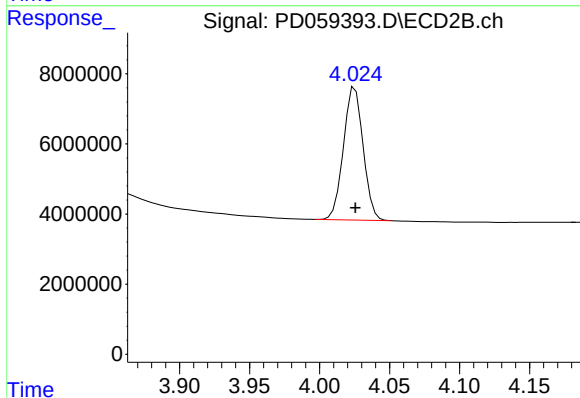


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 37135571
Conc: 22.07 ng/ml

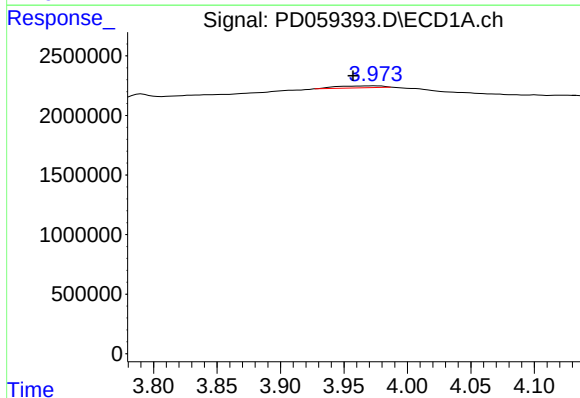


#2 alpha-BHC

R.T.: 3.974 min
Delta R.T.: 0.017 min
Response: 430844
Conc: 0.24 ng/ml

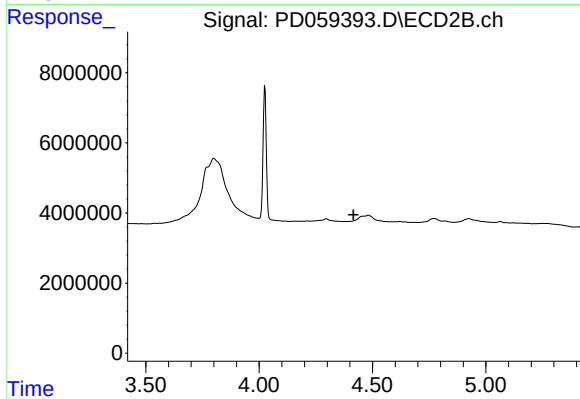

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.416 min
Response: 0
Conc: N.D.

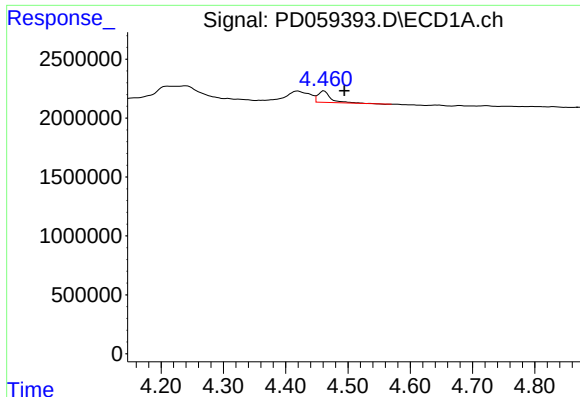

#6 beta-BHC


R.T.: 4.462 min
Delta R.T.: -0.032 min
Response: 1415003
Conc: 1.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

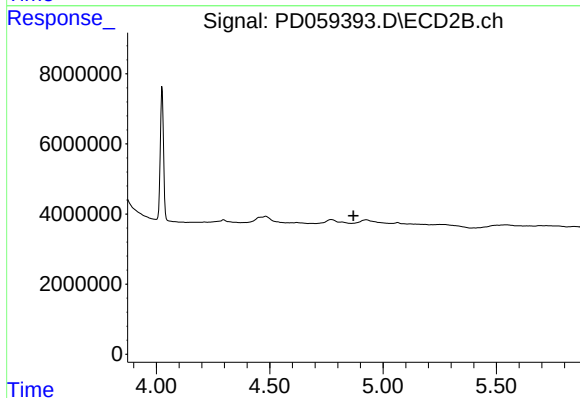


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.870 min
Response: 0
Conc: N.D.

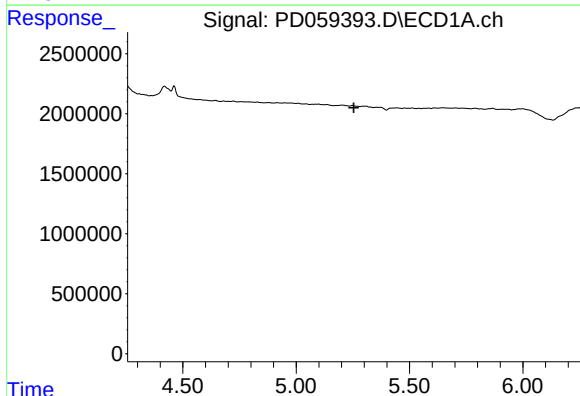


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.254 min
Response: 0
Conc: N.D.

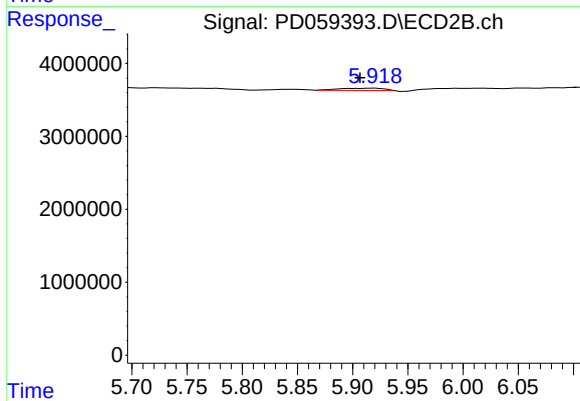

#8 Heptachlor epoxide


R.T.: 5.919 min
Delta R.T.: 0.012 min
Response: 846588
Conc: 0.45 ng/ml

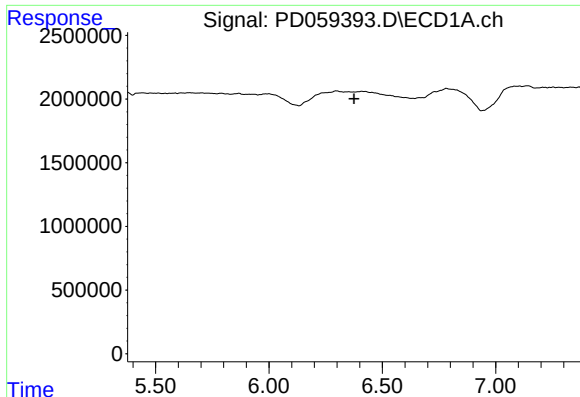

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

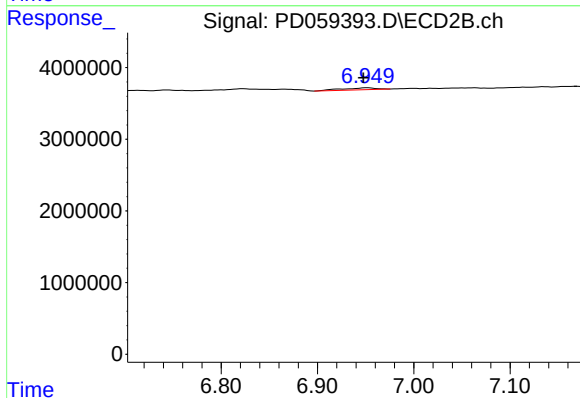


#15 Endosulfan II

R.T.: 6.952 min
Delta R.T.: 0.004 min
Response: 646669
Conc: 0.45 ng/ml

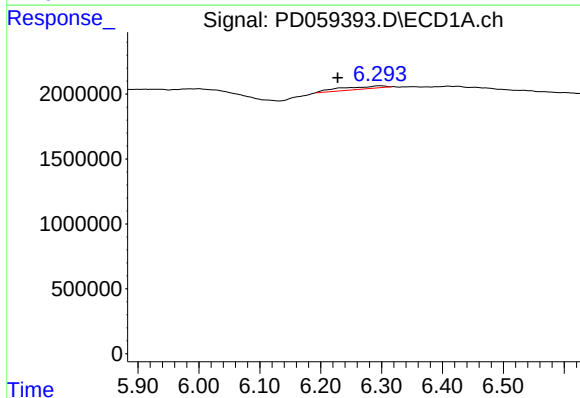


#16 4,4'-DDD

R.T.: 6.296 min
Delta R.T.: 0.068 min
Response: 1061476
Conc: 1.02 ng/ml

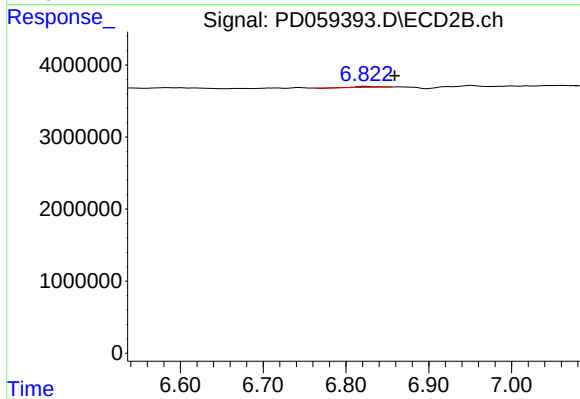

#16 4,4'-DDD


R.T.: 6.823 min
Delta R.T.: -0.036 min
Response: 236237
Conc: 0.17 ng/ml

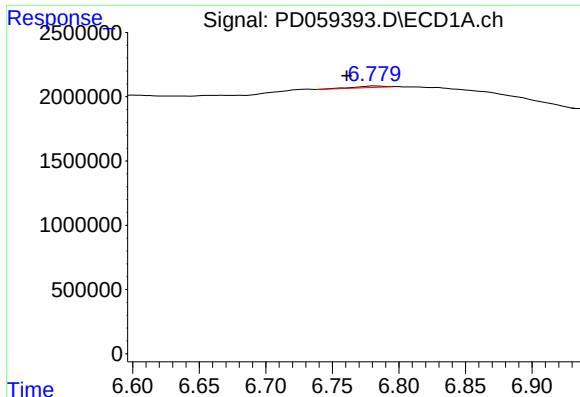

#19 Endosulfan Sulfate


R.T.: 6.782 min
Delta R.T.: 0.022 min
Response: 192541
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

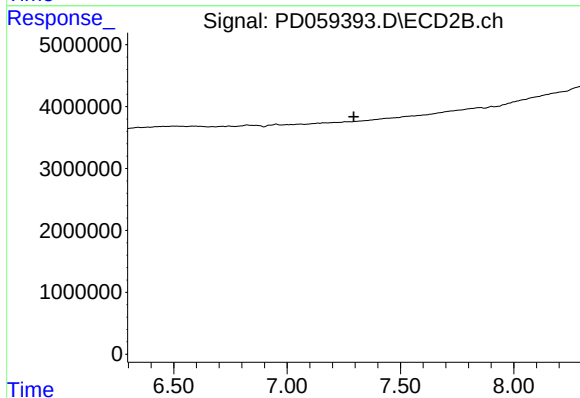


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.295 min
Response: 0
Conc: N.D.

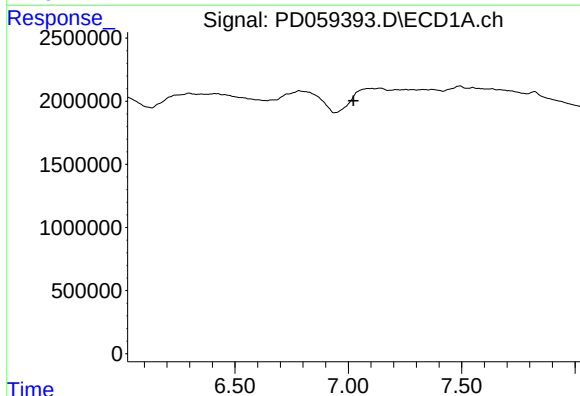


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.023 min
Response: 0
Conc: N.D.

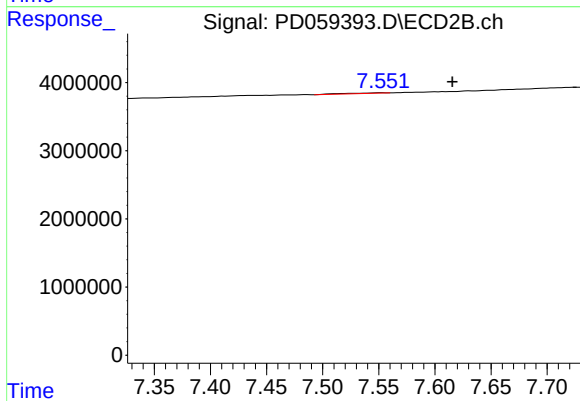

#20 Methoxychlor


R.T.: 7.553 min
Delta R.T.: -0.063 min
Response: 207300
Conc: 0.33 ng/ml

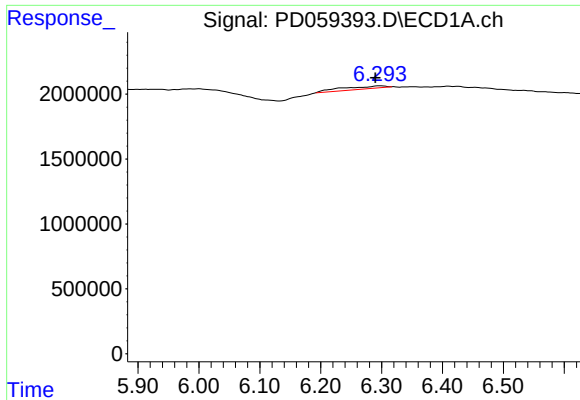

#24 Toxaphene-3


R.T.: 6.296 min
Delta R.T.: 0.006 min
Response: 1061476
Conc: 129.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

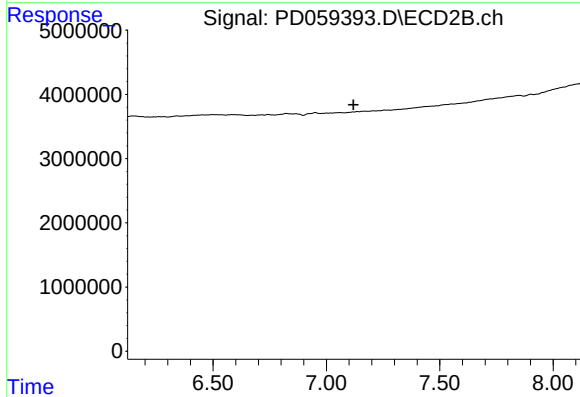


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

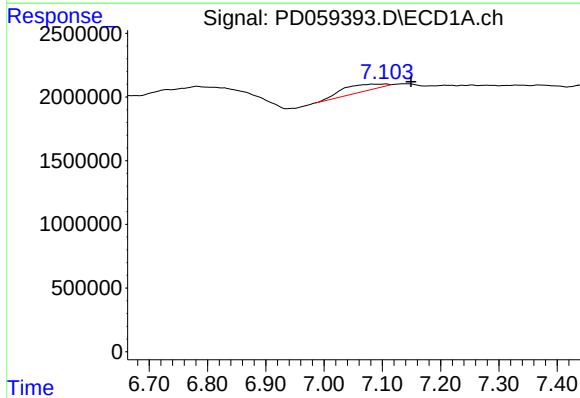


#26 Toxaphene-5

R.T.: 7.106 min
Delta R.T.: -0.043 min
Response: 2669039
Conc: 156.63 ng/ml

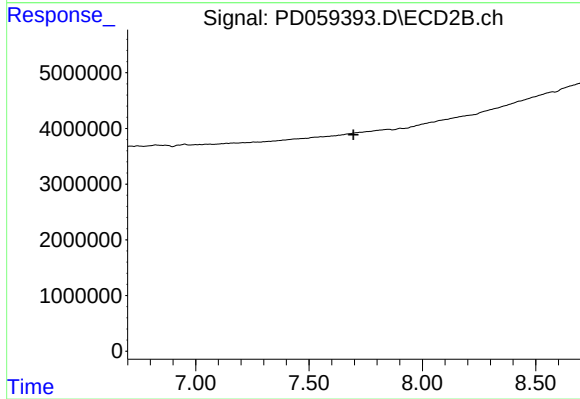

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.696 min
Response: 0
Conc: N.D.

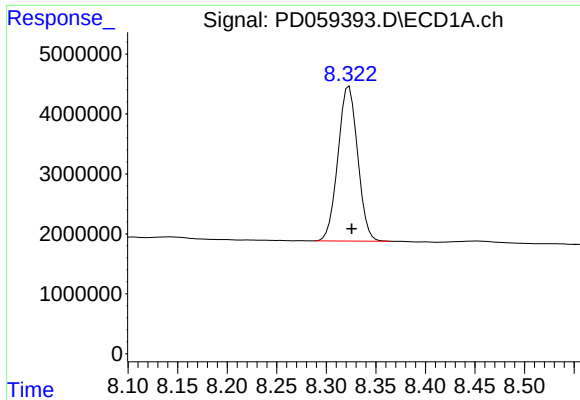

#27 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.003 min
Response: 35720076
Conc: 42.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

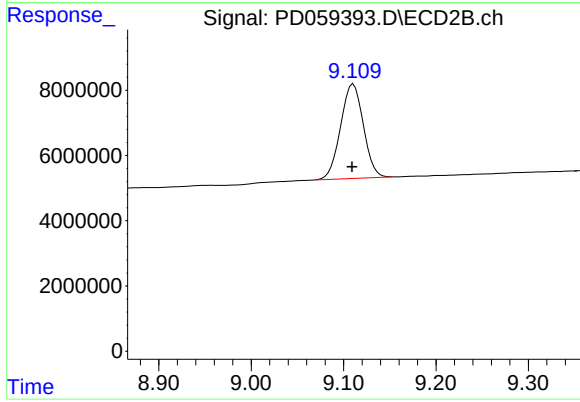

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.001 min
Response: 49715373
Conc: 43.67 ng/ml