

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
 Data File : PD059387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2020 11:17
 Operator : DD\AJ
 Sample : L1955-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-07

Manual Integrations
 APPROVED

Ankita
 9/29/2020 9:38:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 11:43:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.512	4.025	27114823	37244432	21.617	22.134
2)	SA Decachlor...	8.322	9.110	36956797	51115380	43.794	44.902
Target Compounds							
2)	A alpha-BHC	3.955	4.416	2364098	2230778	1.340	0.911 #
3)	MA gamma-BHC...	4.241	4.702	3277910	2492881	1.943	1.114 #
4)	MA Heptachlor	4.551	5.214	2039302	2319003	1.231	1.071
5)	MB Aldrin	4.803	5.521	1920609	2647359	1.188	1.310
6)	B beta-BHC	4.491	4.870	1108739	1125020	1.437	1.113
7)	B delta-BHC	4.700	5.088	1894324	2404934	1.146	1.057
8)	B Heptachlo...	5.251	5.907	1817490	2905469	1.271	1.544
9)	A Endosulfan I	5.593	6.265	1635494	1869981	1.272	1.128
10)	B trans-Chl...	5.480	6.141	1763660	2136169	1.249	1.172
11)	B cis-Chlor...	5.539	6.214	1759377	2077212	1.250	1.151
12)	B 4,4'-DDE	5.704	6.369	1686279	2086168	1.266	1.221
13)	MA Dieldrin	5.839	6.522	1712346	2175999	1.271	1.226
14)	MA Endrin	6.098	6.740	973954	1317927	0.986	1.028m
15)	B Endosulfa...	6.372	6.947	1510093	1984137	1.406m	1.391m
16)	A 4,4'-DDD	6.225	6.860	1539839	1922974	1.482	1.424
17)	MA 4,4'-DDT	6.468	7.157	1347097	1350159	1.279	1.215m
18)	B Endrin al...	6.542	7.071	1330221	1463613	1.501	1.240m
19)	B Endosulfa...	6.757	7.296	1483953	1713219	1.461	1.176
20)	A Methoxychlor	7.024	7.616	514183	779003	1.043	1.257
21)	B Endrin ke...	7.252	7.769	1597149	1819143	1.483	1.299

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
Data File : PD059387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2020 11:17
Operator : DD\AJ
Sample : L1955-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 11:43:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

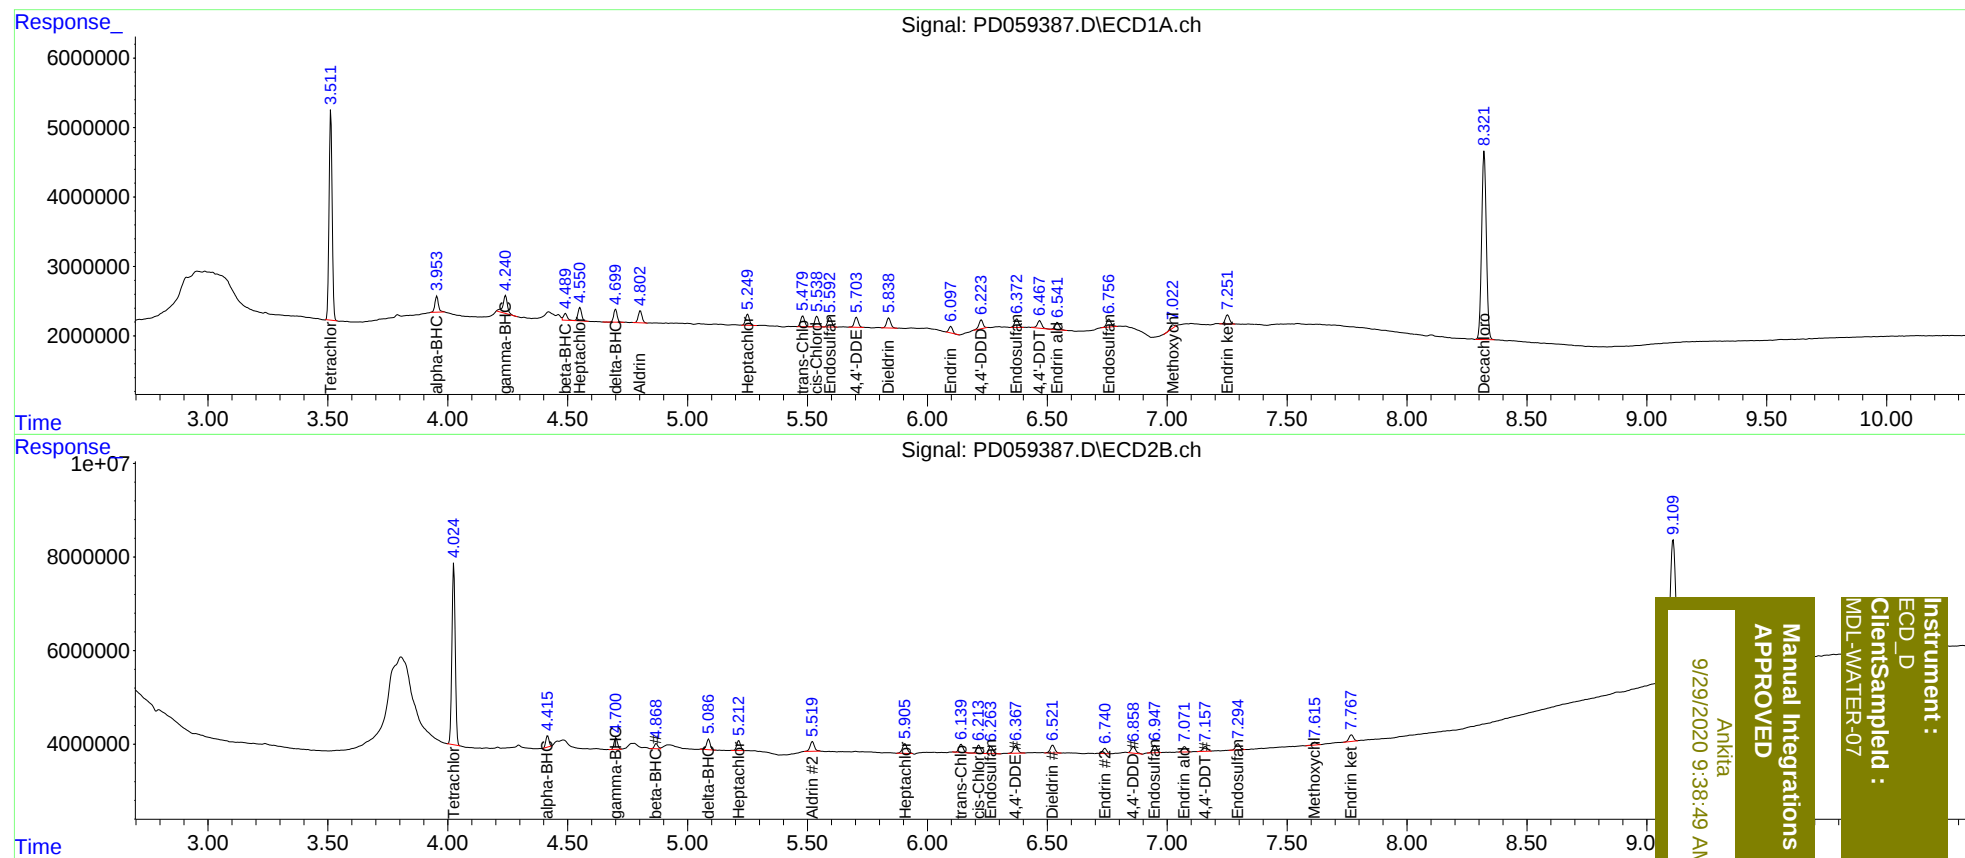

Manual Integrations
APPROVED

Ankita
9/29/2020 9:38:49 AM

Instrument :
ECD_D
Client Sample :
MDL-WATER-07