

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
 Data File : PD059400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2020 17:15
 Operator : DD\AJ
 Sample : BS TEST 5/10 PPB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BS TEST 5/10 PPB

Manual Integrations
 APPROVED

Ankita
 9/29/2020 11:23:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 08:52:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.025	28619003	40245012	22.816	23.917
2)	SA Decachlor...	8.324	9.112	38882390	52913377	46.076	46.481
Target Compounds							
2)	A alpha-BHC	3.955	4.415	10024230	12076816	5.683	4.933
3)	MA gamma-BHC...	4.242	4.701	9527672	12105785	5.647	5.412
4)	MA Heptachlor	4.551	5.213	9252272	11378595	5.587	5.254
5)	MB Aldrin	4.804	5.520	8937025	11241928	5.529	5.562
6)	B beta-BHC	4.492	4.868	4244568	5377347	5.500	5.318
7)	B delta-BHC	4.701	5.087	8613071	11884884	5.210	5.226
8)	B Heptachlo...	5.251	5.906	8273255	11154843	5.785	5.928
9)	A Endosulfan I	5.595	6.264	7444114	9348325	5.788	5.640
10)	B trans-Chl...	5.481	6.140	8082339	10119464	5.722	5.552
11)	B cis-Chlor...	5.541	6.214	7908558	9909211	5.617	5.488
12)	B 4,4'-DDE	5.706	6.368	14622417	18587017	10.979	10.883
13)	MA Dieldrin	5.841	6.522	14810070	19508280	10.989	10.988
14)	MA Endrin	6.100	6.740	10569732	13262428	10.702	10.341
15)	B Endosulfa...	6.375	6.948	12309494	17350048	11.457	12.161
16)	A 4,4'-DDD	6.226	6.859	12342857	17606968	11.878	13.040
17)	MA 4,4'-DDT	6.470	7.158	11576556	12951809	10.995	11.654
18)	B Endrin al...	6.544	7.072	11007906	12651775	12.421	10.717
19)	B Endosulfa...	6.759	7.295	11533610	15160375	11.359	10.404
20)	A Methoxychlor	7.021	7.615	27051826	34121879	54.869	55.053
21)	B Endrin ke...	7.254	7.766	13916867	16960300	12.925	12.115m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
Data File : PD059400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2020 17:15
Operator : DD\AJ
Sample : BS TEST 5/10 PPB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 08:52:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

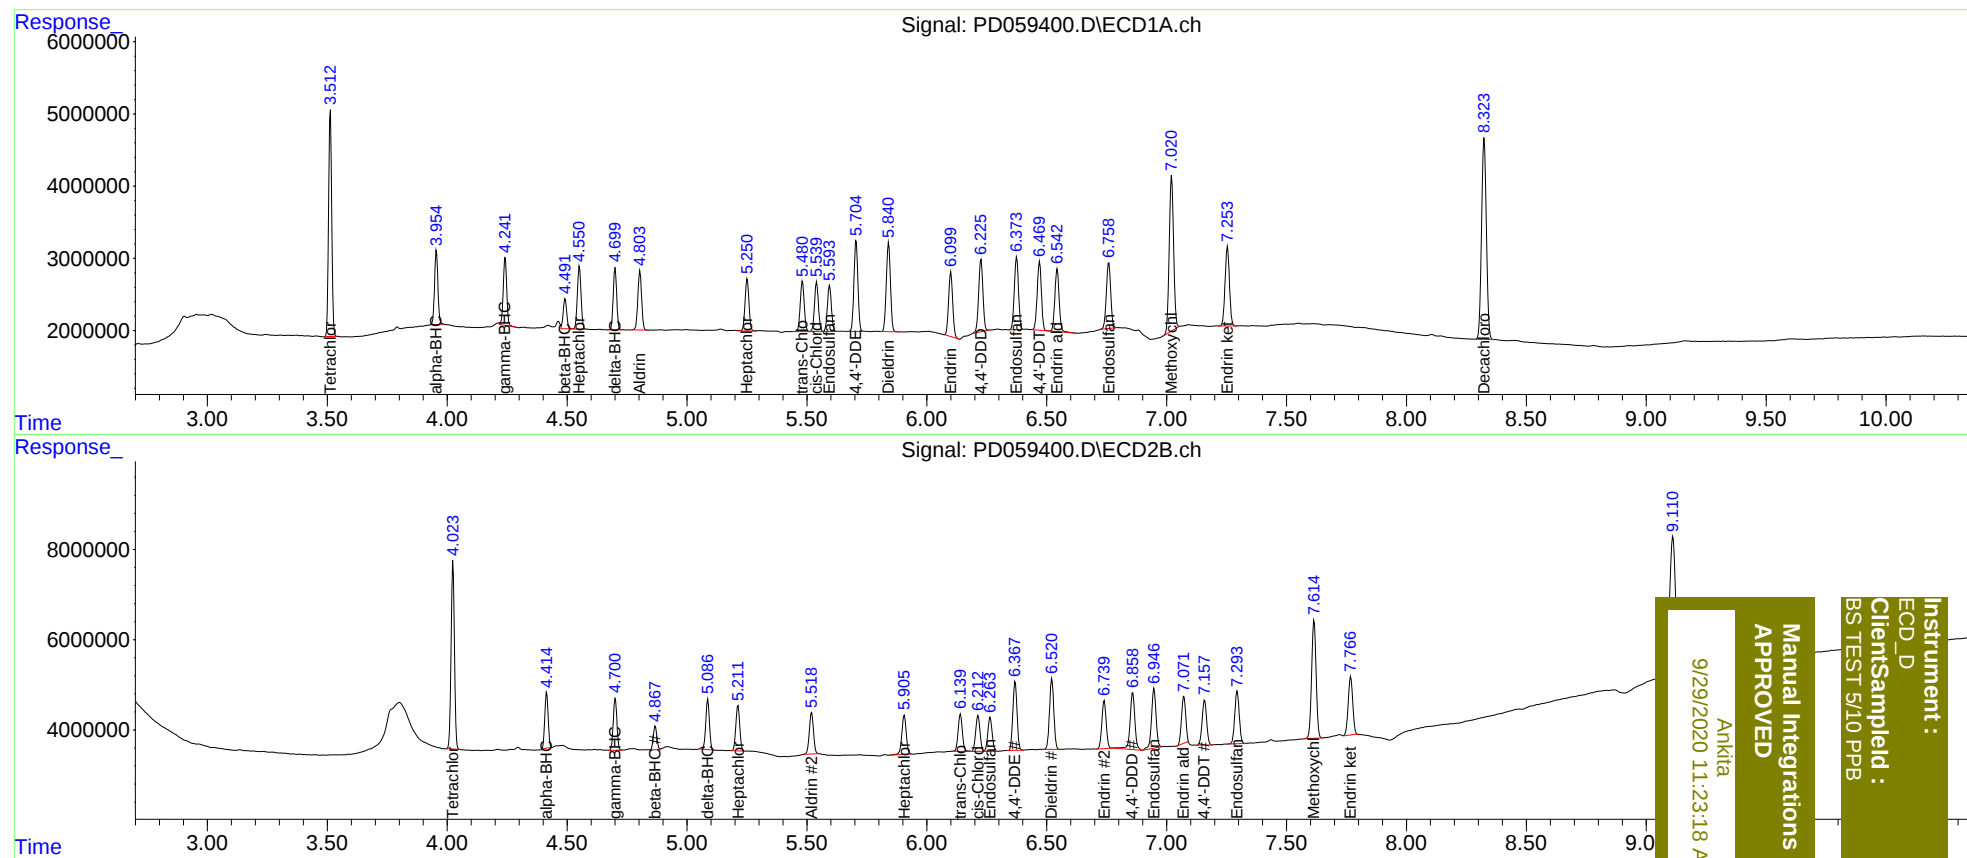

Manual Integrations
APPROVED

Ankita
9/29/2020 11:23:18 AM

Instrument :
ECD_D
ClientSample :
BS TEST 5/10 PPB