

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
 Data File : PD059386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2020 11:03
 Operator : DD\AJ
 Sample : L1955-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-06

Manual Integrations
 APPROVED

Ankita
 9/29/2020 9:38:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 11:43:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	26434080	36371619	21.074	21.615
27)	SA Decachlor...	8.323	9.111	36276175	49589606	42.988	43.562
Target Compounds							
2)	A alpha-BHC	3.955	4.417	2423672	2120460	1.374	0.866 #
3)	MA gamma-BHC...	4.241	4.702	3316685	2412118	1.966	1.078 #
4)	MA Heptachlor	4.552	5.214	2019542	2210100	1.219	1.020
5)	MB Aldrin	4.803	5.521	1832736	2470768	1.134	1.222
6)	B beta-BHC	4.491	4.870	1070651	910018	1.387	0.900 #
7)	B delta-BHC	4.700	5.088	1784053	2382469	1.079	1.048
8)	B Heptachlo...	5.251	5.908	1735341	2381555	1.213	1.266
9)	A Endosulfan I	5.594	6.265	1670261	1916245	1.299	1.156
10)	B trans-Chl...	5.481	6.141	1779500	2015709	1.260	1.106
11)	B cis-Chlor...	5.540	6.214	1722611	1926468	1.223	1.067
12)	B 4,4'-DDE	5.705	6.370	1643481	1881537	1.234	1.102
13)	MA Dieldrin	5.840	6.522	1600257	2080044	1.187	1.172
14)	MA Endrin	6.099	6.741	933860	1227823	0.946	0.957
15)	B Endosulfa...	6.373	6.947	1446636	1924259	1.346	1.349m
16)	A 4,4'-DDD	6.225	6.860	1541175	1918185	1.483	1.421
17)	MA 4,4'-DDT	6.469	7.159	1256669	1326578	1.194	1.194
18)	B Endrin al...	6.543	7.072	1191876	1412622	1.345	1.197
19)	B Endosulfa...	6.758	7.296	1362649	1721057	1.342	1.181
20)	A Methoxychlor	7.022	7.617	617438	802359	1.252m	1.295
21)	B Endrin ke...	7.253	7.768	1449003	1681786	1.346	1.201

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092820\
Data File : PD059386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2020 11:03
Operator : DD\AJ
Sample : L1955-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 11:43:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

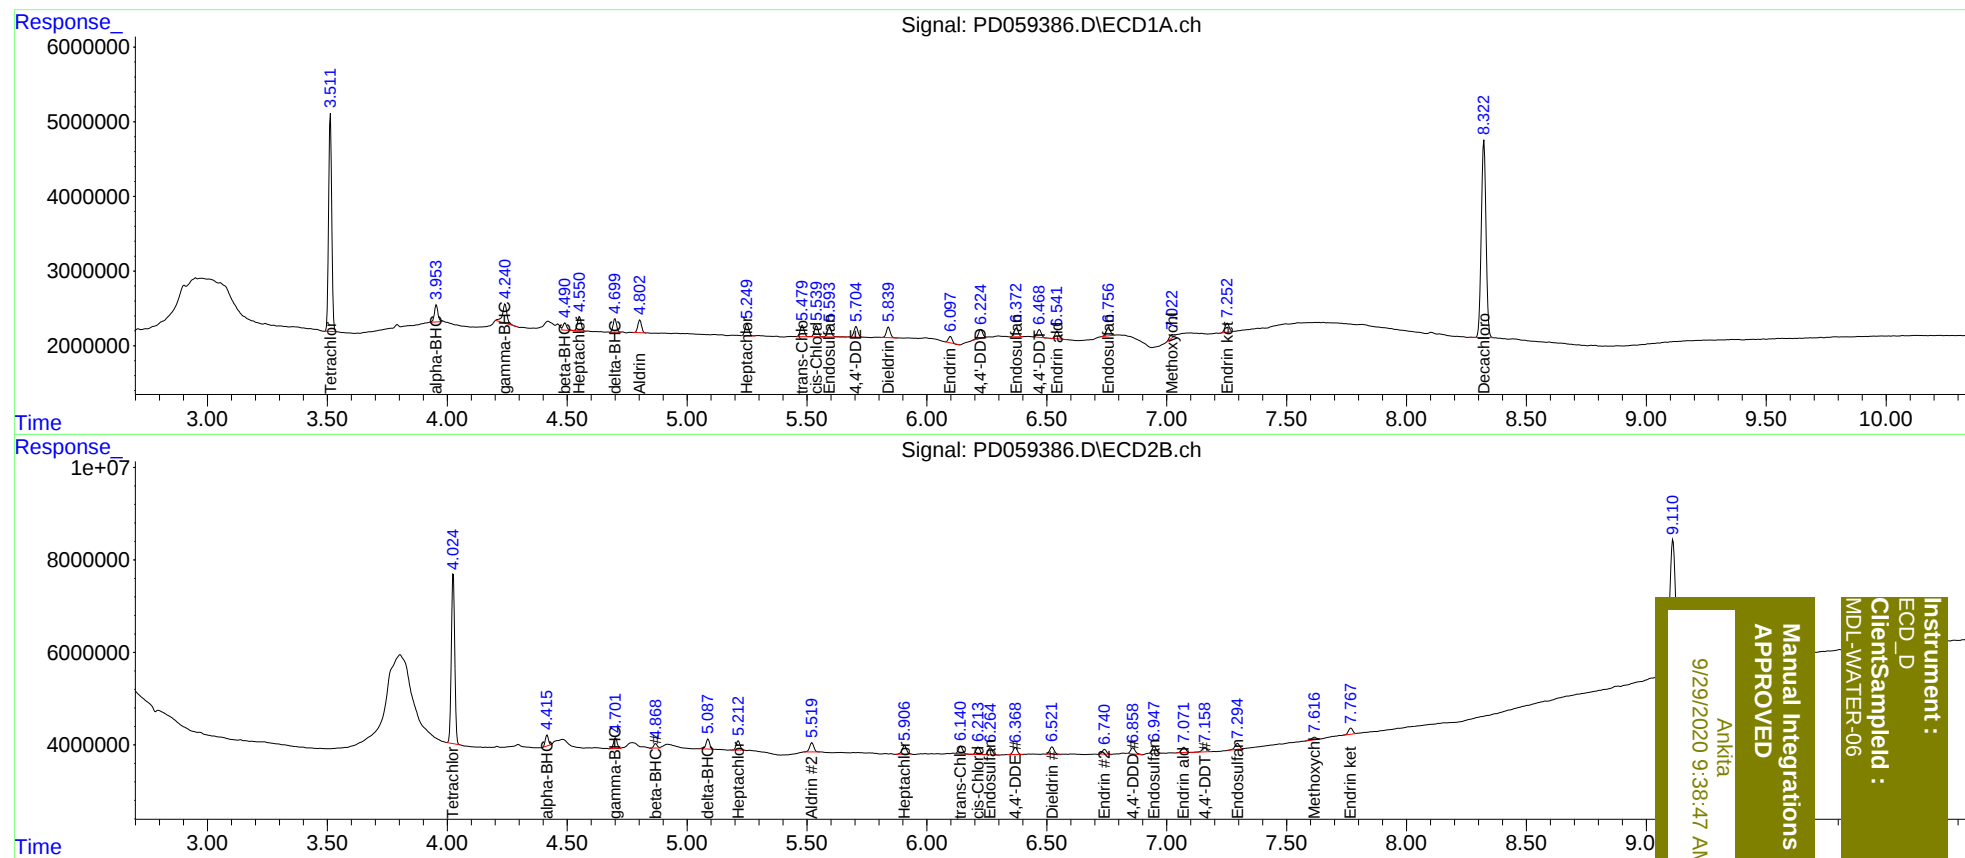

Manual Integrations
APPROVED

Ankita
9/29/2020 9:38:47 AM

Instrument :
ECD_D
Client Sample :
MDL-WATER-06