

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092821\
 Data File : PD065943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2021 12:12
 Operator : AR\AJ
 Sample : M3917-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

mohammad
 9/29/2021 9:32:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 16:19:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.493	4.012	16286058	125.2E6	21.992	21.799
28) SA Decachlor...	8.233	9.087	25494449	104.2E6	18.664m	26.926 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092821\
Data File : PD065943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2021 12:12
Operator : AR\AJ
Sample : M3917-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

mohammad
9/29/2021 9:32:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 16:19:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

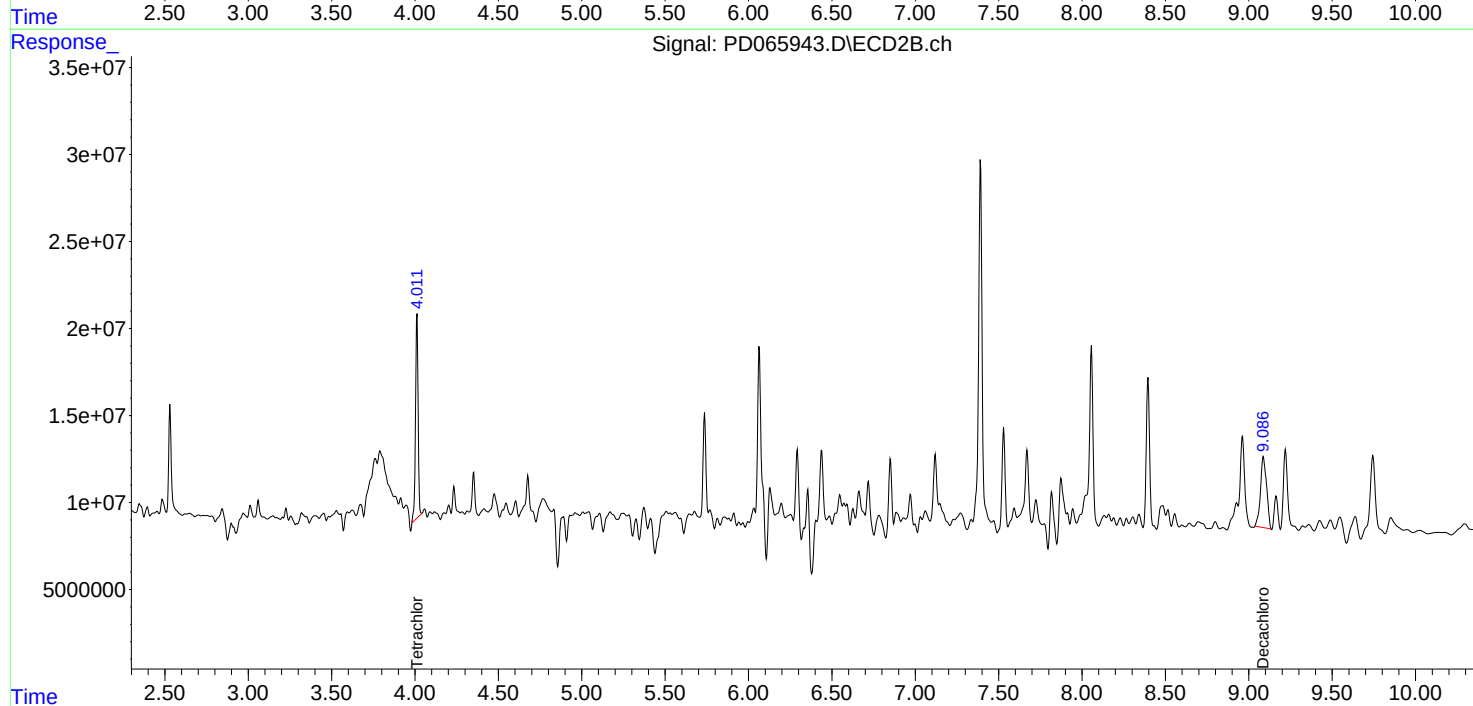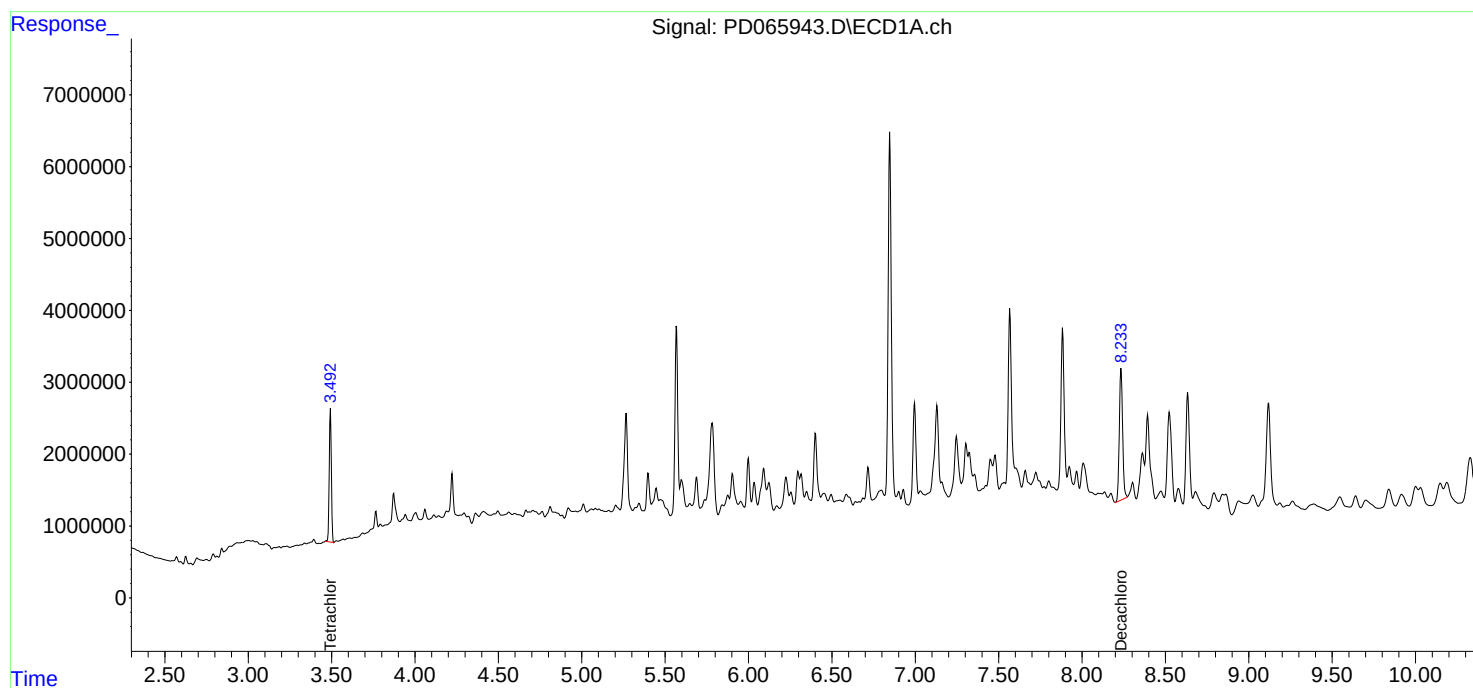

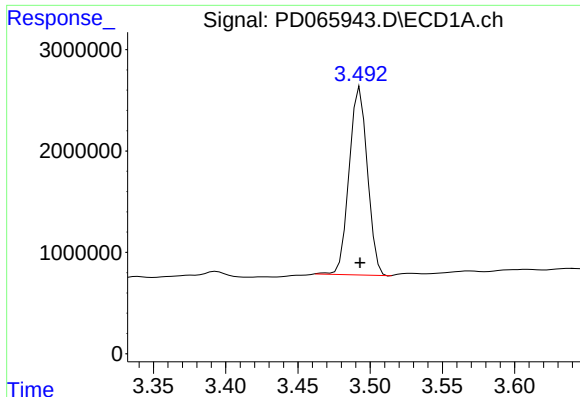


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 16286058
Conc: 21.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

mohammad
9/29/2021 9:32:08 AM

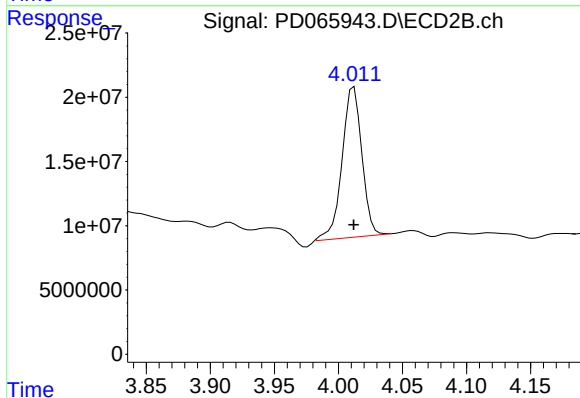


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 125175441
Conc: 21.80 ng/ml

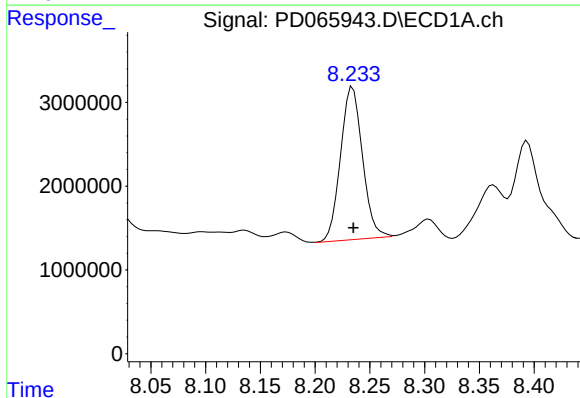

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: -0.002 min
Response: 25494449
Conc: 18.66 ng/ml m

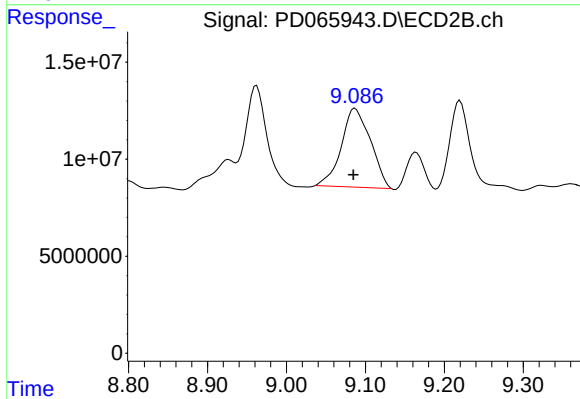

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.002 min
Response: 104206112
Conc: 26.93 ng/ml