

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
 Data File : PD072072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 11:16
 Operator : AR\AJ
 Sample : PB147927BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS927

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 04:34:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.811	3.563	43256138	572.5E6	17.061	18.583
2)	SA Decachlor...	7.997	9.089	87166906	333.4E6	37.181	37.216
Target Compounds							
2)	A alpha-BHC	3.319	4.029	16206110	209.3E6	4.376	4.919
3)	MA gamma-BHC...	3.653	4.365	15898073	188.5E6	4.546	5.327
4)	MA Heptachlor	3.999	4.942	15254721	144.6E6	4.293	5.734 #
5)	MB Aldrin	4.282	5.284	16201215	124.6E6	4.559	5.670
6)	B beta-BHC	3.952	4.572	6326547	78846375	3.953	5.299 #
7)	B delta-BHC	4.185	4.819	13429261	124.1E6	3.792	4.981 #
8)	B Heptachlo...	4.789	5.716	15275455	99891424	4.798	6.551 #
9)	A Endosulfan I	5.162	6.104	14112693	85158106	5.008	5.713
10)	B trans-Chl...	5.041	5.971	15559691	92259708	4.764	5.339
11)	B cis-Chlor...	5.106	6.049	15550554	90915124	4.846	5.401
12)	B 4,4'-DDE	5.296	6.222	26288914	162.3E6	8.882	10.816
13)	MA Dieldrin	5.429	6.382	29981028	172.1E6	9.752	11.396
14)	MA Endrin	5.706	6.614	25184950	128.9E6	9.499	10.456
15)	B Endosulfa...	6.000	6.840	25544477	138.9E6	10.235	11.436
16)	A 4,4'-DDD	5.854	6.746	23344480	130.8E6	9.999	11.324
17)	MA 4,4'-DDT	6.107	7.057	22669937	127.3E6	9.462	11.191
18)	B Endrin al...	6.181	6.971	20382262	106.3E6	9.386	10.255
19)	B Endosulfa...	6.405	7.203	23810909	118.1E6	9.435	10.253
20)	A Methoxychlor	6.686	7.534	66087688	292.5E6	51.424	56.267
21)	B Endrin ke...	6.914	7.695	30339385	143.5E6	10.728	11.489
22)	Toxaphene-1	5.429f	0.000	29981028	0	1907.841	N.D. #
23)	Toxaphene-2	5.706f	6.222f	25184950	162.3E6	1499.949	2201.756 #
24)	Toxaphene-3	6.000	7.057f	25544477	127.3E6	1339.713	684.748 #
25)	Toxaphene-4	6.825	7.203	653300	118.1E6	8.338	464.952 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
Data File : PD072072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 11:16
Operator : AR\AJ
Sample : PB147927BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 04:34:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

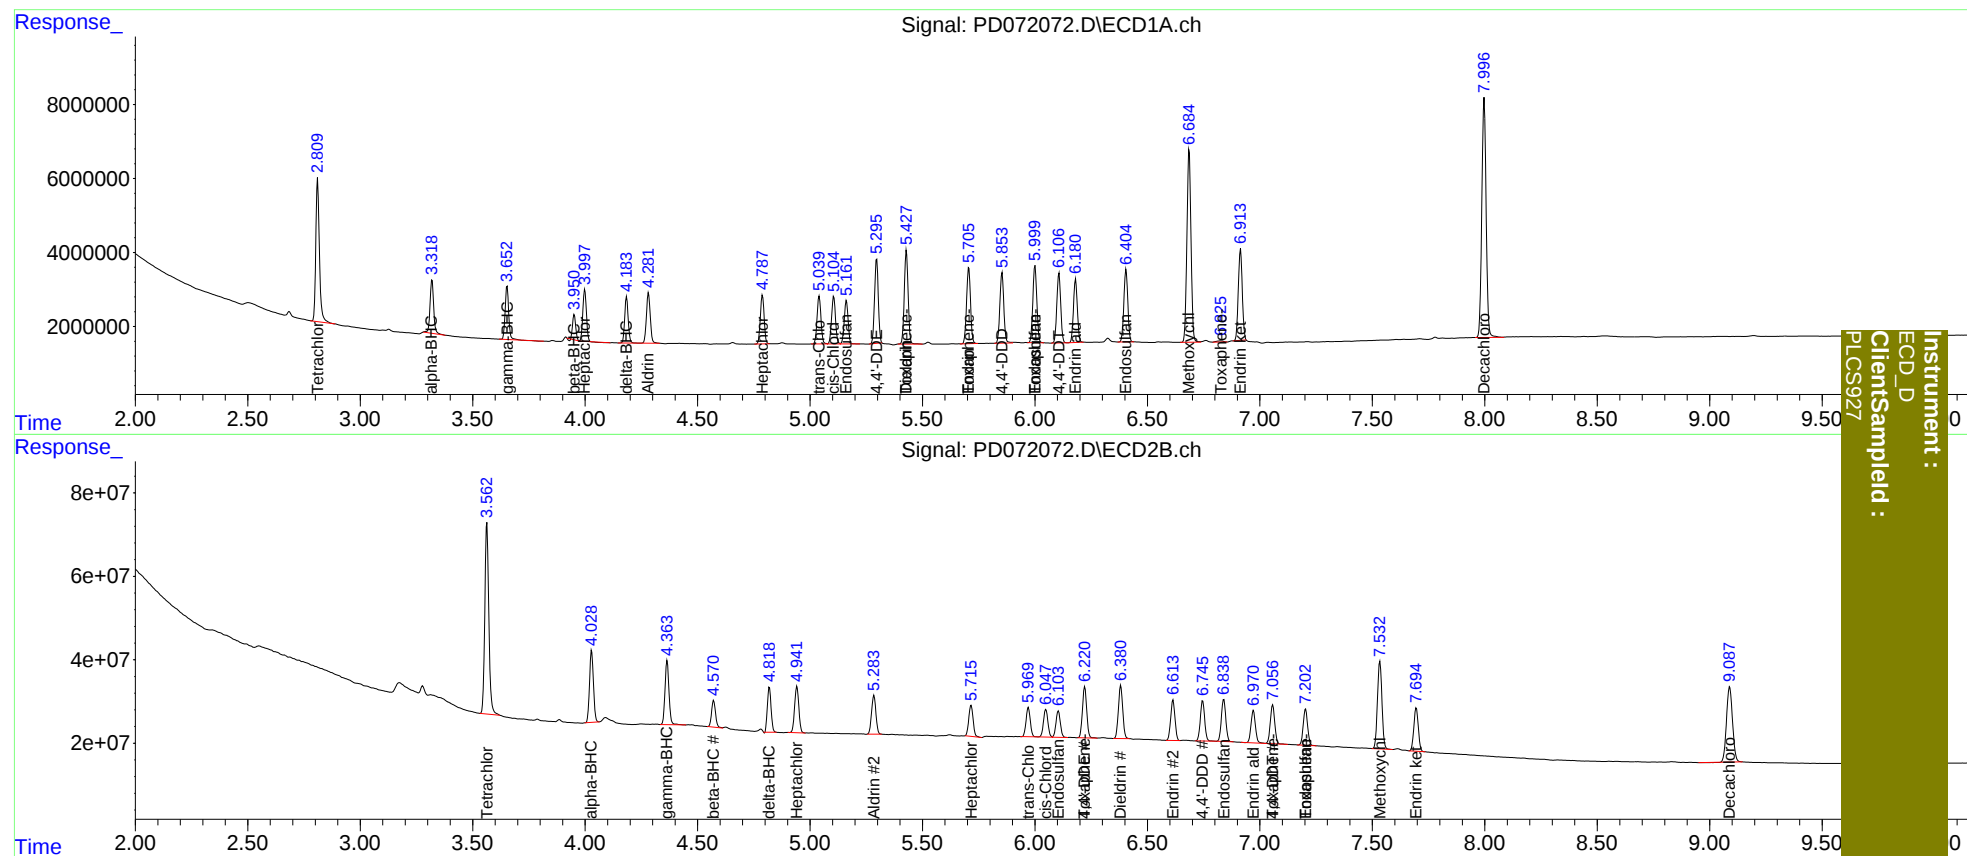

Instrument :
ECD_D
ClientSampled :
PLCS927