

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
 Data File : PD072073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 11:46
 Operator : AR\AJ
 Sample : N4745-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 04:34:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.811	3.561	28735487	324.1E6	11.334	10.519
27)	SA Decachlor...	7.998	9.068	58334400	704.7E6	24.882	78.673 #
Target Compounds							
2)	A alpha-BHC	3.314	3.990f	-1563051	19166236	N.D.	0.451
3)	MA gamma-BHC...	3.659	0.000	180.5E6	0	51.619	N.D. #
4)	MA Heptachlor	4.011	0.000	5548933	0	1.562	N.D. #
5)	MB Aldrin	4.263	0.000	1984838	0	0.558	N.D. #
6)	B beta-BHC	3.913f	4.585	872437	149.3E6	0.545	10.038 #
7)	B delta-BHC	4.178	4.837	16085533	52724767	4.543	2.116 #
8)	B Heptachlo...	4.789	5.711	1414023	11548188	0.444	0.757 #
9)	A Endosulfan I	5.189	6.047f	149.9E6	226.5E6	53.176	15.193 #
10)	B trans-Chl...	5.042	5.971	12665302	2079.7E6	3.878	120.350 #
11)	B cis-Chlor...	5.106	6.047	18233220	226.5E6	5.682	13.455 #
12)	B 4,4'-DDE	5.306	6.216	3764479	84123207	1.272	5.606 #
13)	MA Dieldrin	5.433	6.384	70061734	62203672	22.788	4.120 #
14)	MA Endrin	5.703	6.660f	13147992	130.8E6	4.959	10.610 #
15)	B Endosulfa...	6.007	6.833	27331953	78290974	10.952	6.445 #
16)	A 4,4'-DDD	5.852	6.747	25587191	291.0E6	10.960	25.191 #
17)	MA 4,4'-DDT	6.103	7.036	5909489	100.8E6	2.466	8.856 #
18)	B Endrin al...	6.199	6.965	2921134	88597787	1.345	8.544 #
19)	B Endosulfa...	6.424	0.000	8770441	0	3.475	N.D. #
20)	A Methoxychlor	6.716	7.523	162.5E6	45025419	126.466	8.661 #
21)	B Endrin ke...	6.856f	0.000	116.3E6	0	41.139	N.D. #
22)	Toxaphene-1	5.403	5.902	321.1E6	735.4E6	20431.447	12739.717 #
23)	Toxaphene-2	5.745	6.216f	3568680	84123207	212.541	1141.212 #
24)	Toxaphene-3	6.007	7.036f	27331953	100.8E6	1433.459	541.879 #
25)	Toxaphene-4	6.757f	0.000	2706577	0	34.545	N.D. #
26)	Toxaphene-5	0.000	7.600	0	427.0E6	N.D.	2836.783

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
Data File : PD072073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 11:46
Operator : AR\AJ
Sample : N4745-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 04:34:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

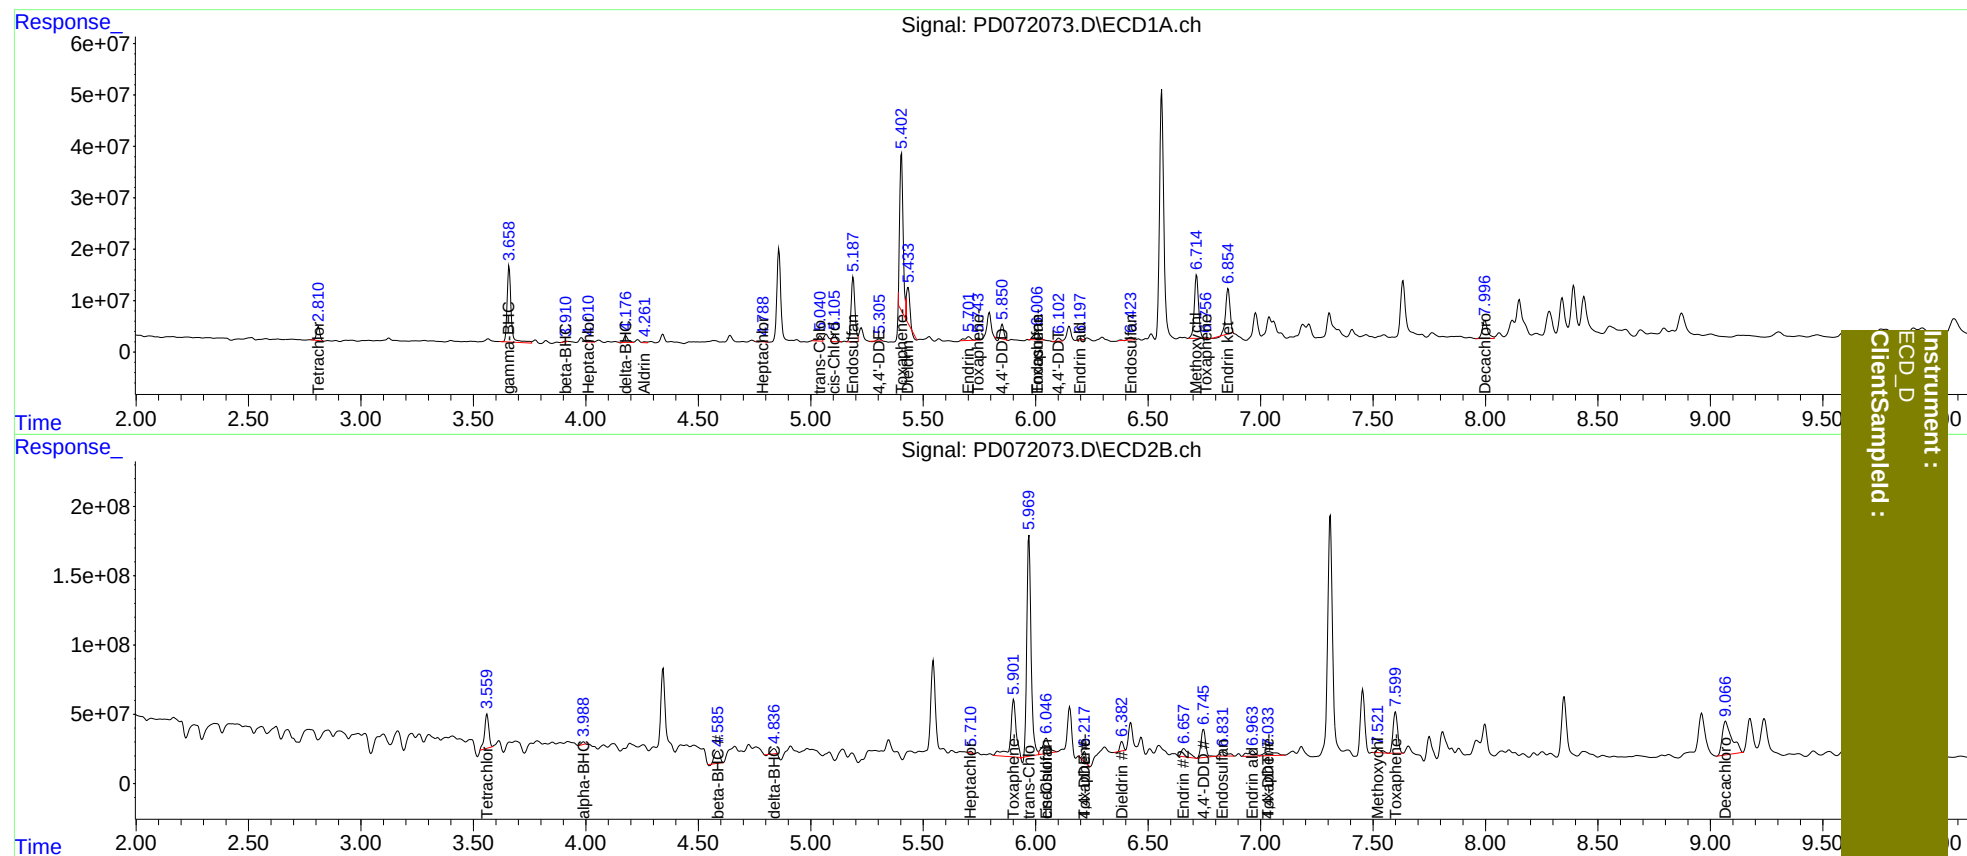

Instrument :
ECD_D
ClientSampled :
0