

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
 Data File : PD072088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 17:57
 Operator : AR\AJ
 Sample : N4824-06MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8P3MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 04:39:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.564	38331809	465.4E6	15.119	15.104
27)	SA Decachlor...	7.991	9.087	56466993	185.0E6	24.086	20.658
Target Compounds							
2)	A alpha-BHC	3.313	4.030	130.7E6	1114.0E6	35.288	26.185 #
3)	MA gamma-BHC...	3.646	4.365	85705081	1136.1E6	24.510	32.112 #
4)	MA Heptachlor	3.992	4.942	141.2E6	758.9E6	39.738	30.091
5)	MB Aldrin	4.275	5.283	137.3E6	687.9E6	38.621	31.302
6)	B beta-BHC	3.944	4.571	54309586	422.2E6	33.932	28.378
7)	B delta-BHC	4.178	4.819	75557754	486.2E6	21.338	19.512
8)	B Heptachlo...	4.781	5.715	123.0E6	497.9E6	38.629	32.655
9)	A Endosulfan I	5.154	6.103	113.7E6	481.4E6	40.360	32.297
10)	B trans-Chl...	5.034	5.970	126.7E6	520.5E6	38.792	30.124
11)	B cis-Chlor...	5.098	6.047	121.7E6	517.8E6	37.936	30.763
12)	B 4,4'-DDE	5.289	6.220	235.0E6	937.9E6	79.383	62.504
13)	MA Dieldrin	5.459	6.379	2641524	1247.4E6	0.859	82.612 #
14)	MA Endrin	5.699	6.613	287.0E6	877.7E6	108.262	71.202 #
15)	B Endosulfa...	5.993	6.838	206.3E6	644.6E6	82.645	53.060 #
16)	A 4,4'-DDD	5.847	6.744	173.2E6	793.8E6	74.195	68.722
17)	MA 4,4'-DDT	6.100	7.056	202.8E6	806.1E6	84.622	70.843
18)	B Endrin al...	6.174	6.969	154.7E6	498.2E6	71.253	48.041 #
19)	B Endosulfa...	6.398	7.202	179.0E6	701.1E6	70.929	60.851
20)	A Methoxychlor	6.679	7.532	569.7E6	1958.0E6	443.310	376.645
21)	B Endrin ke...	6.908	7.693	233.5E6	877.9E6	82.569	70.292
22)	Toxaphene-1	5.422	0.000	258.7E6	0	16464.515	N.D. #
23)	Toxaphene-2	5.790f	6.220f	2908594	937.9E6	173.228	12724.039 #
24)	Toxaphene-3	5.993f	7.107	206.3E6	4072420	10817.310	21.901 #
25)	Toxaphene-4	6.791	7.202	930210	701.1E6	11.873	2759.364 #
26)	Toxaphene-5	7.074f	7.620	854565	10127704	25.552	67.278 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
Data File : PD072088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 17:57
Operator : AR\AJ
Sample : N4824-06MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 04:39:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

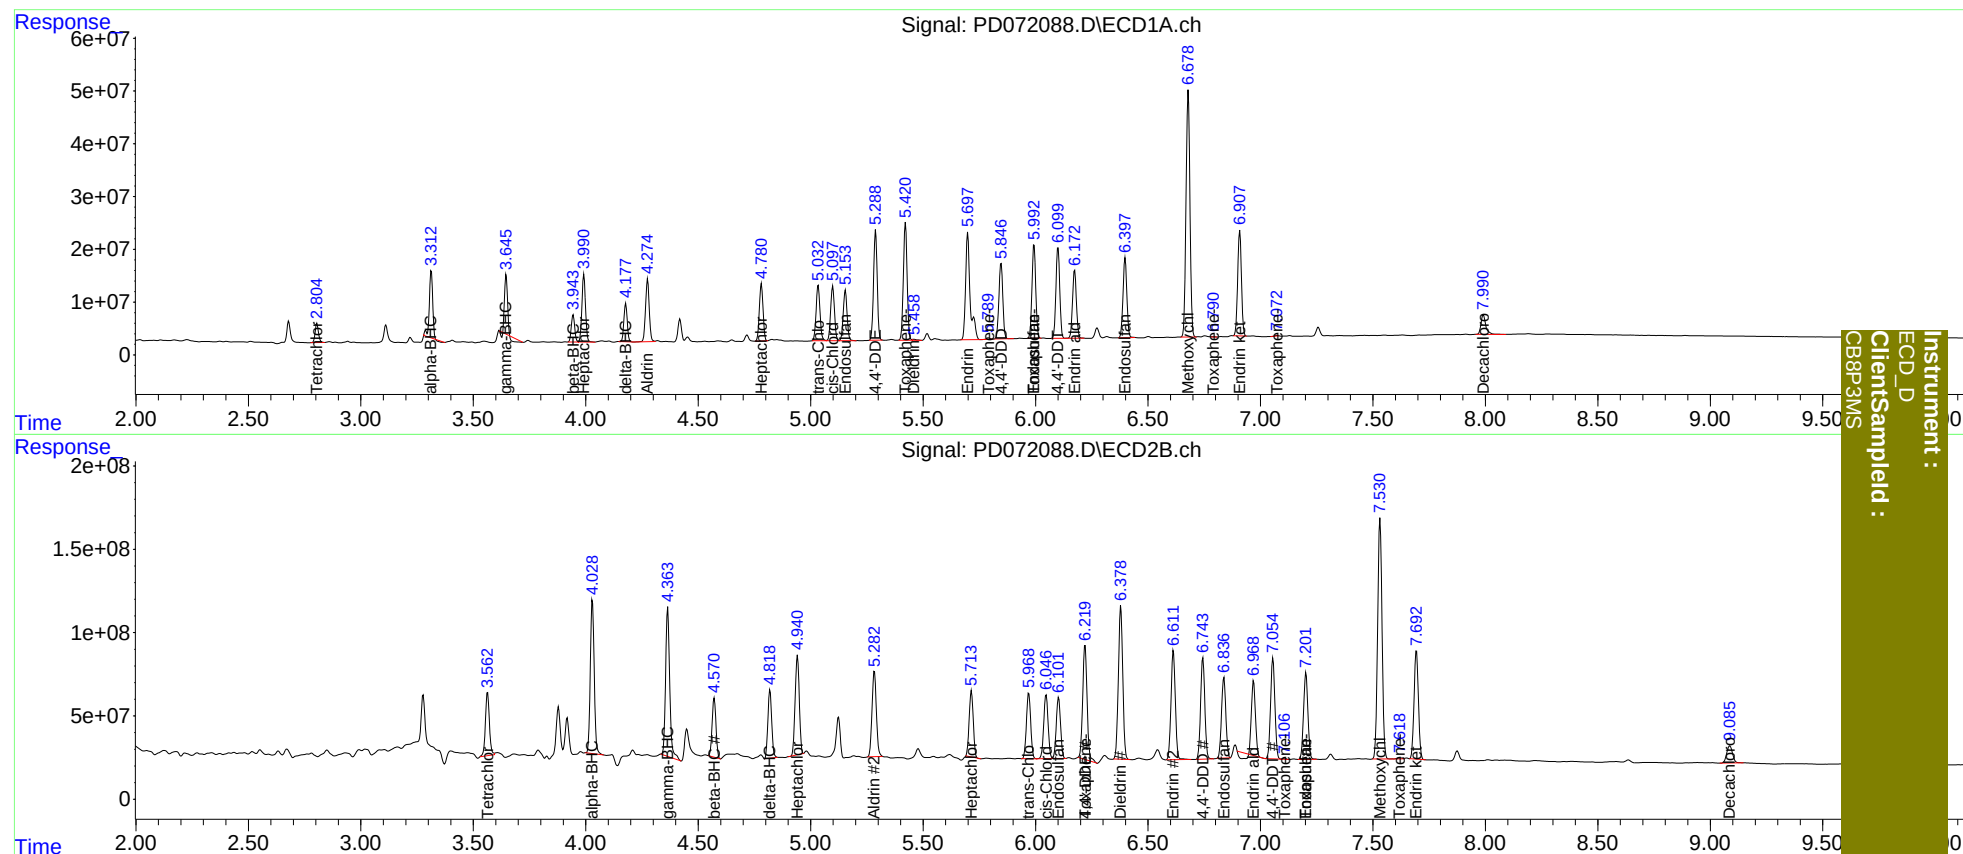

Instrument :
ECD_D
ClientSampled :
CB8P3MS