

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
 Data File : PD072076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 12:26
 Operator : AR\AJ
 Sample : N4745-04MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8N7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/29/2022
 Supervised By : Ankita Jodhani 09/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 04:35:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.562	29585529	394.7E6	11.669	12.812m
27)	SA Decachlor...	7.991	9.065	52205630	400.4E6	22.268	44.697m#
Target Compounds							
2)	A alpha-BHC	3.313	4.027	185.2E6	1880.8E6	50.020	44.209m
3)	MA gamma-BHC...	3.645	4.363	207.7E6	1687.4E6	59.400m	47.696m
4)	MA Heptachlor	3.992	4.941	182.7E6	1077.0E6	51.411	42.702
5)	MB Aldrin	4.274	5.283	179.1E6	905.0E6	50.408m	41.183
6)	B beta-BHC	3.944	4.571	71325128	653.7E6	44.563	43.935m
7)	B delta-BHC	4.178	4.819	110.9E6	708.9E6	31.309	28.448
8)	B Heptachlo...	4.781	5.713	152.1E6	689.2E6	47.789	45.203m
9)	A Endosulfan I	5.155	6.101	128.3E6	625.5E6	45.513m	41.958m
10)	B trans-Chl...	5.034	5.969	181.2E6	1439.3E6	55.472	83.294m#
11)	B cis-Chlor...	5.099	6.045	174.9E6	794.9E6	54.516	47.223m
12)	B 4,4'-DDE	5.289	6.219	285.3E6	1131.6E6	96.384	75.412
13)	MA Dieldrin	5.421	6.379	384.9E6	1398.6E6	125.195m	92.625m#
14)	MA Endrin	5.699	6.611	277.8E6	1043.4E6	104.784	84.639m
15)	B Endosulfa...	5.993	6.840	251.0E6	1409.0E6	100.585m	115.984
16)	A 4,4'-DDD	5.847	6.744	232.1E6	1085.4E6	99.423	93.970
17)	MA 4,4'-DDT	6.099	7.054	243.1E6	1039.0E6	101.464m	91.318m
18)	B Endrin al...	6.175	6.968	193.2E6	851.2E6	88.973	82.080m
19)	B Endosulfa...	6.399	7.202	204.0E6	865.9E6	80.818	75.160
20)	A Methoxychlor	6.679	7.532	669.1E6	2280.7E6	520.620	438.726
21)	B Endrin ke...	6.908	7.694	248.2E6	1011.4E6	87.774	80.988

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
Data File : PD072076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 12:26
Operator : AR\AJ
Sample : N4745-04MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 04:35:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

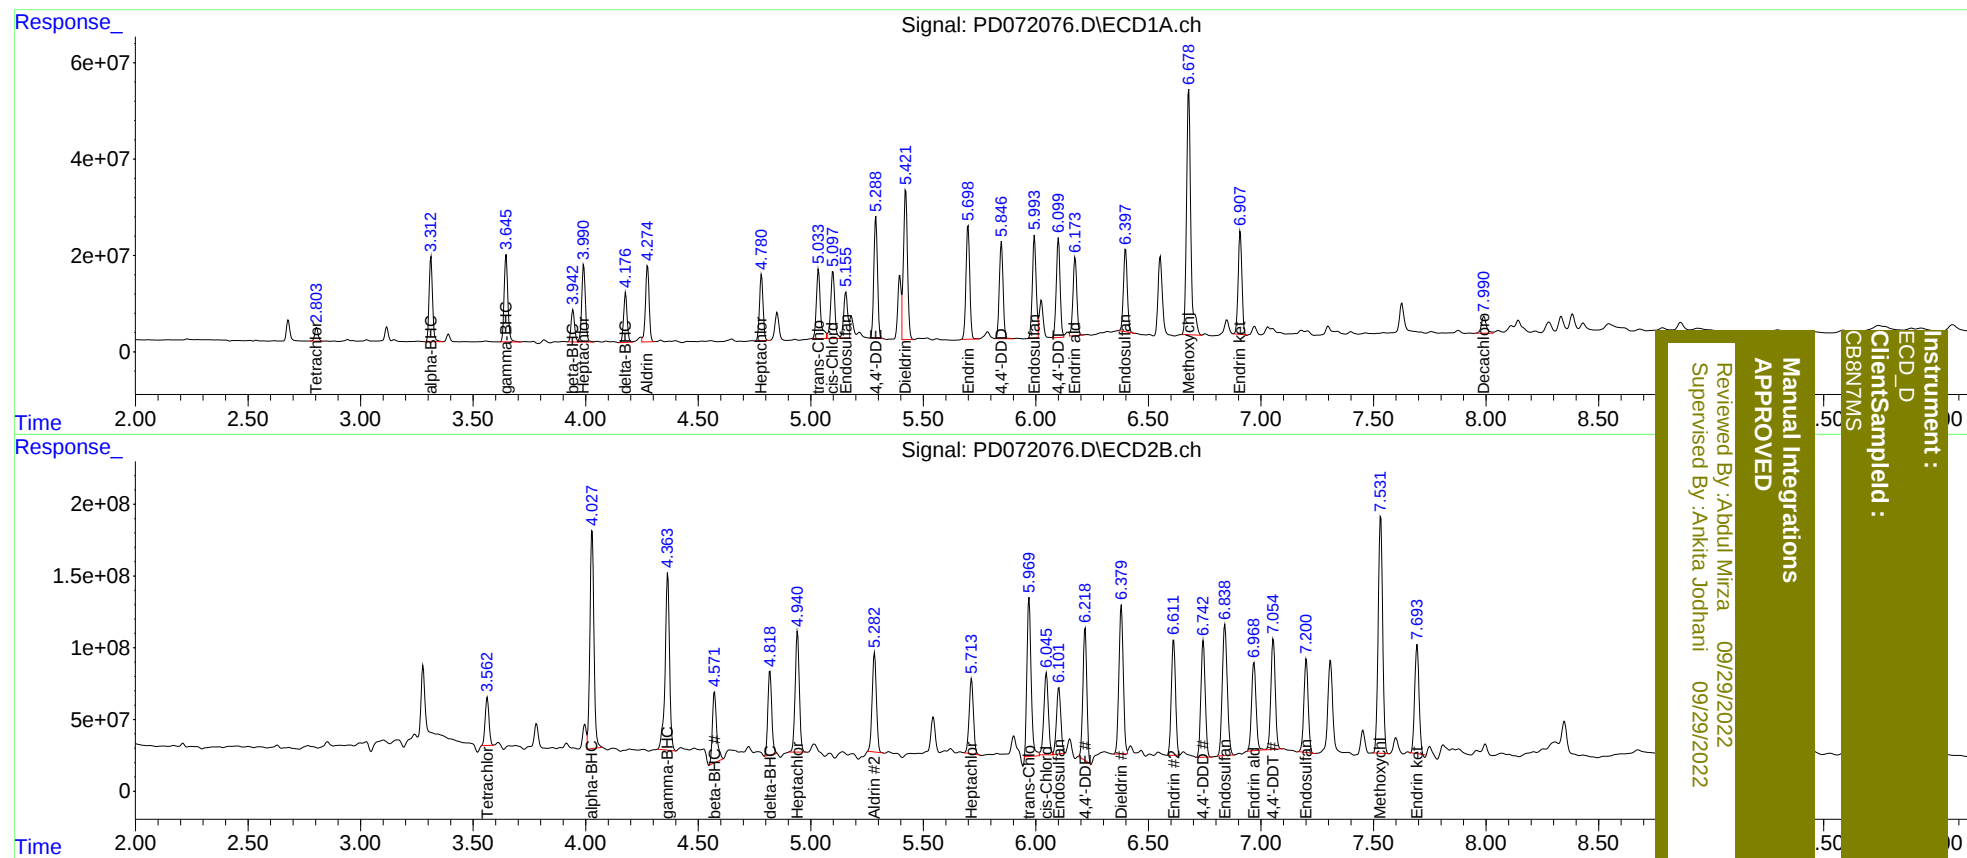

Reviewed By: Abdul Mirza 09/29/2022
Supervised By: Ankita Jodhani 09/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
CB8N7MS