

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
 Data File : PD072077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 12:39
 Operator : AR\AJ
 Sample : N4745-05MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8N7MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/29/2022
 Supervised By : Ankita Jodhani 09/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 04:35:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.562	29478642	389.1E6	11.627	12.630m
2)	SA Decachlor...	7.991	9.066	50465552	447.6E6	21.526	49.974m#
Target Compounds							
2)	A alpha-BHC	3.313	4.027	184.3E6	1876.1E6	49.753	44.099m
3)	MA gamma-BHC...	3.645	4.363	206.2E6	1680.9E6	58.978m	47.509m
4)	MA Heptachlor	3.992	4.941	181.2E6	1080.0E6	50.996	42.824
5)	MB Aldrin	4.273	5.284	176.8E6	896.9E6	49.758m	40.816
6)	B beta-BHC	3.944	4.571	70663247	657.3E6	44.149	44.176m
7)	B delta-BHC	4.177	4.818	110.6E6	763.8E6	31.238	30.651m
8)	B Heptachlo...	4.781	5.715	151.4E6	669.6E6	47.546	43.912
9)	A Endosulfan I	5.154	6.103	127.3E6	623.4E6	45.157m	41.820
10)	B trans-Chl...	5.033	5.969	178.0E6	1405.0E6	54.515	81.310m#
11)	B cis-Chlor...	5.098	6.046	166.3E6	765.7E6	51.832	45.487m
12)	B 4,4'-DDE	5.289	6.219	282.0E6	1130.5E6	95.283	75.336
13)	MA Dieldrin	5.420	6.379	384.5E6	1387.1E6	125.068m	91.861m#
14)	MA Endrin	5.699	6.612	276.7E6	1061.0E6	104.360	86.066
15)	B Endosulfa...	5.994	6.840	243.8E6	1393.0E6	97.680	114.670
16)	A 4,4'-DDD	5.847	6.744	232.2E6	1077.0E6	99.451	93.240
17)	MA 4,4'-DDT	6.098	7.056	241.5E6	1088.9E6	100.789m	95.698
18)	B Endrin al...	6.174	6.968	194.1E6	845.4E6	89.392	81.526m
19)	B Endosulfa...	6.399	7.202	205.8E6	867.0E6	81.568	75.253
20)	A Methoxychlor	6.680	7.532	663.4E6	2256.5E6	516.237	434.070
21)	B Endrin ke...	6.908	7.694	246.7E6	1041.8E6	87.251	83.420

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092822\
Data File : PD072077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 12:39
Operator : AR\AJ
Sample : N4745-05MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 04:35:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

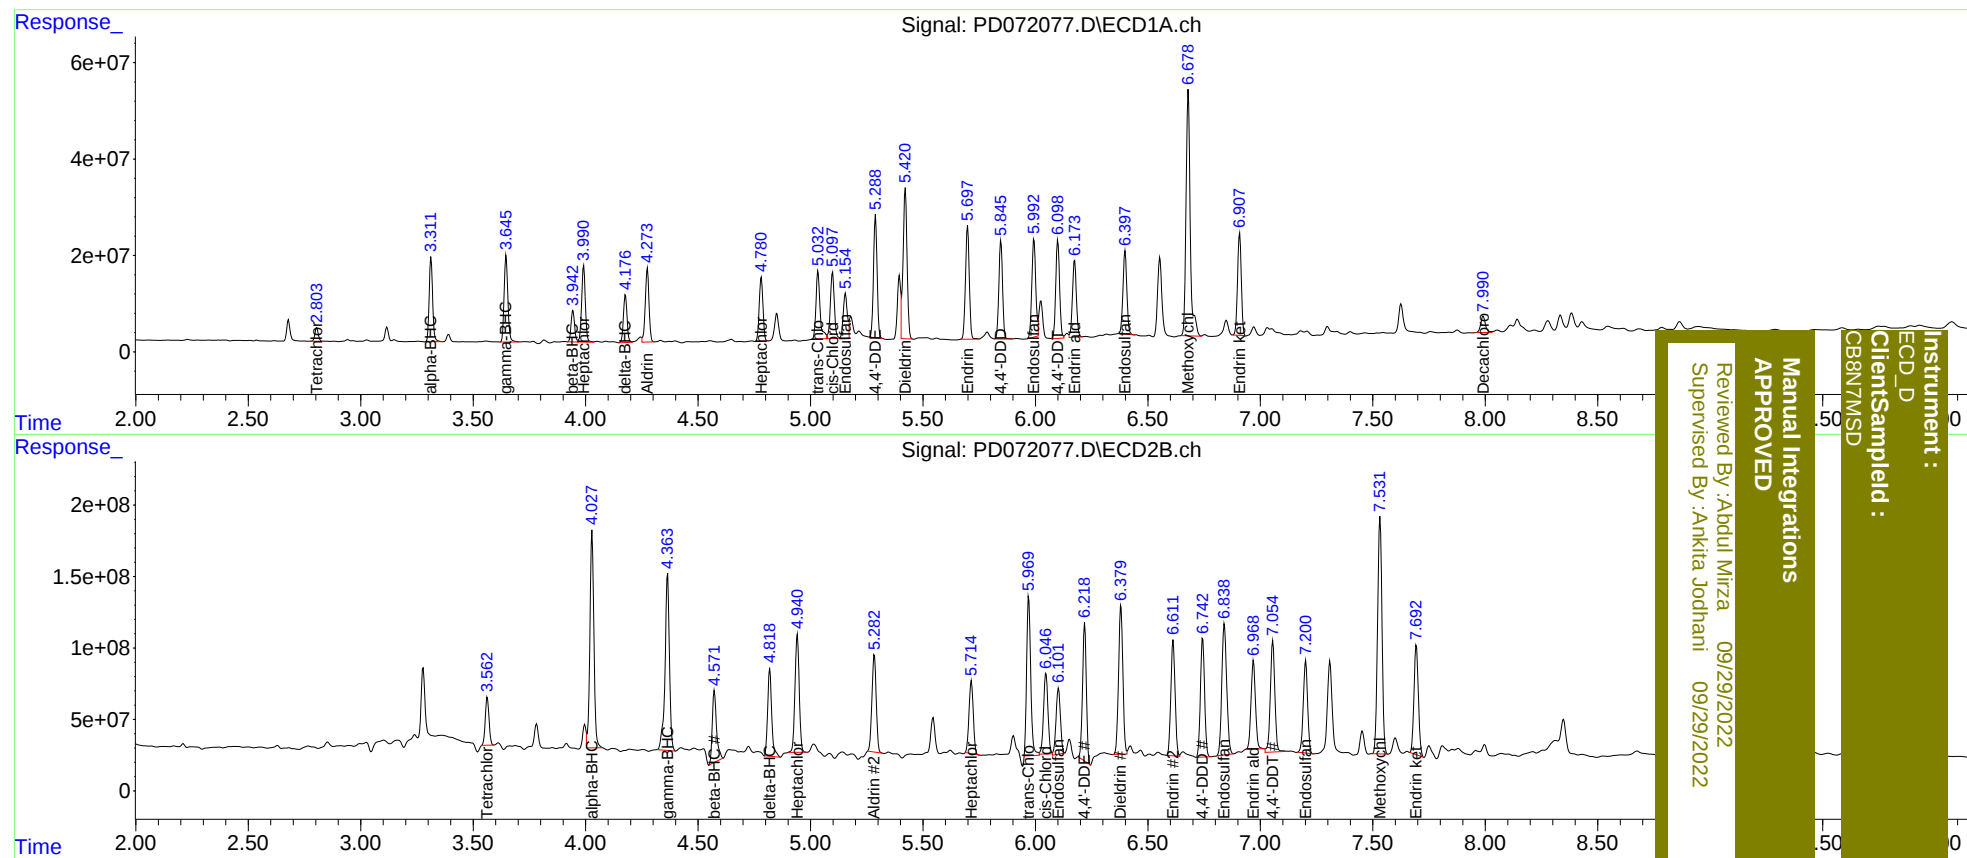

Reviewed By: Abdul Mirza 09/29/2022
Supervised By: Ankita Jodhani 09/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
CB8N7MSD