

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092822\  
 Data File : PD072079.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Sep 2022 13:07  
 Operator : AR\AJ  
 Sample : INDA326  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3182

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 09/29/2022  
 Supervised By : Ankita Jodhani 09/29/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 29 04:35:54 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD092422CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Sep 23 17:46:27 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 2.807 | 3.563 | 47258090 | 594.4E6 | 18.639  | 19.292  |
| 27)                         | SA Decachlor... | 7.993 | 9.086 | 77610200 | 298.2E6 | 33.105m | 33.295m |
| Target Compounds            |                 |       |       |          |         |         |         |
| 2)                          | A alpha-BHC     | 3.315 | 4.029 | 69792128 | 804.7E6 | 18.845  | 18.915  |
| 3)                          | MA gamma-BHC... | 3.648 | 4.364 | 65456294 | 665.4E6 | 18.719  | 18.807  |
| 4)                          | MA Heptachlor   | 3.994 | 4.942 | 66124439 | 483.3E6 | 18.610  | 19.162  |
| 9)                          | A Endosulfan I  | 5.156 | 6.103 | 51103804 | 272.8E6 | 18.134m | 18.301  |
| 13)                         | MA Dieldrin     | 5.424 | 6.380 | 113.7E6  | 551.0E6 | 36.967  | 36.493  |
| 14)                         | MA Endrin       | 5.701 | 6.613 | 94170231 | 435.9E6 | 35.519  | 35.362  |
| 16)                         | A 4,4'-DDD      | 5.849 | 6.745 | 87407771 | 429.6E6 | 37.441  | 37.190  |
| 17)                         | MA 4,4'-DDT     | 6.103 | 7.056 | 79994923 | 392.2E6 | 33.387  | 34.467  |
| 20)                         | A Methoxychlor  | 6.682 | 7.532 | 226.3E6  | 895.8E6 | 176.123 | 172.316 |
| -----                       |                 |       |       |          |         |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092822\  
Data File : PD072079.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Sep 2022 13:07  
Operator : AR\AJ  
Sample : INDA326  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 29 04:35:54 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD092422CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Sep 23 17:46:27 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

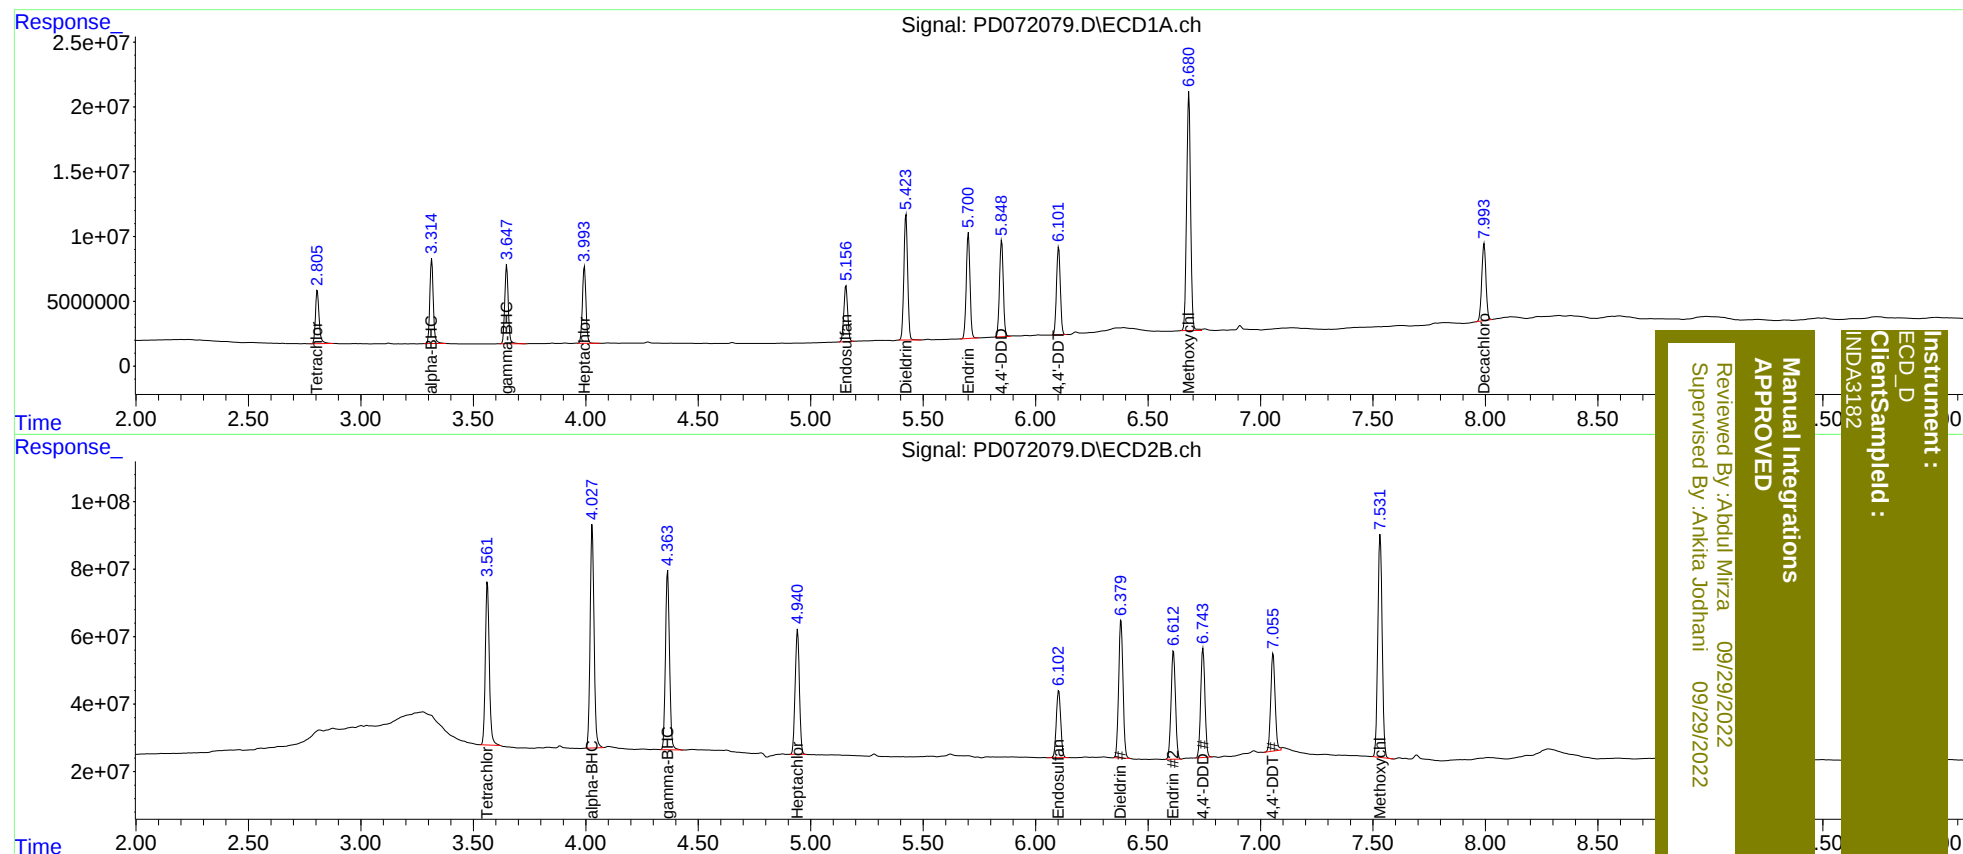

Reviewed By: Abdul Mirza 09/29/2022  
Supervised By: Ankita Jodhani 09/29/2022

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
Client Sampled :  
INDA3182