

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092823\
 Data File : PD078436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 14:01
 Operator : AR\AJ
 Sample : 04480-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBJY5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/29/2023
 Supervised By : Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 03:03:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.759	45937029	27367638	18.708	16.566
2) SA Decachlor...	9.077	7.893	63975369	35275114	19.791	19.054
Target Compounds						
5) MB Aldrin	5.260	4.220	3017505	650640	0.742	0.265 #
9) A Endosulfan I	6.078	5.099	1034238	783543	0.310m	0.381

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092823\
Data File : PD078436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 14:01
Operator : AR\AJ
Sample : 04480-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 03:03:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

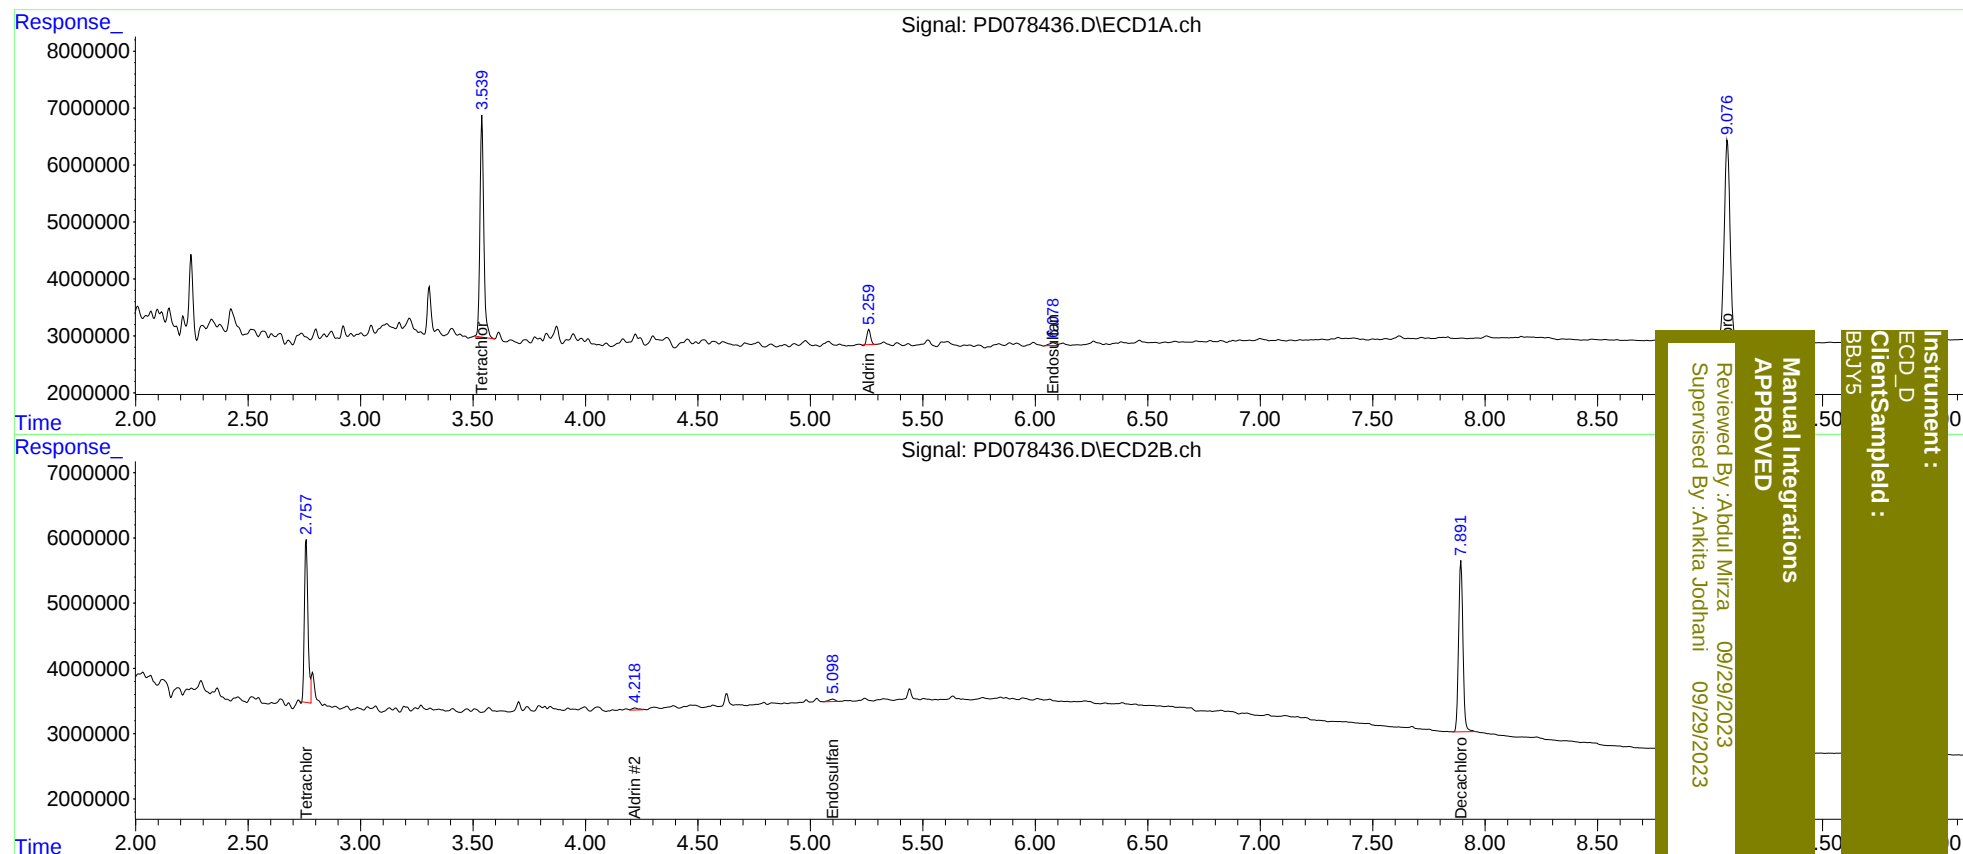

Reviewed By: Abdul Mirza 09/29/2023
Supervised By: Ankita Jodhani 09/29/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BBJY5