

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 12:07
 Operator : AR\AJ
 Sample : P4019-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCB0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/29/2024
 Supervised By : Ankita Jodhani 09/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 13:44:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	2.890	29810342	6859.3E6	28.455m	1620.034m#
2)	SA Decachlor...	8.874	8.071	30466252	29154040	20.667m	7.540m#
Target Compounds							
2)	A alpha-BHC	3.887	3.388	534.0E6	953.6E6	293.394	147.636 #
7)	B delta-BHC	4.644	4.252	714.1E6	1314.4E6	403.469	220.460 #
11)	B cis-Chlor...	5.892	5.187	24323371	115.6E6	15.597m	20.924 #
14)	MA Endrin	6.423	5.782	221.9E6	169.6E6	184.833	37.799m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 12:07
Operator : AR\AJ
Sample : P4019-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 13:44:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

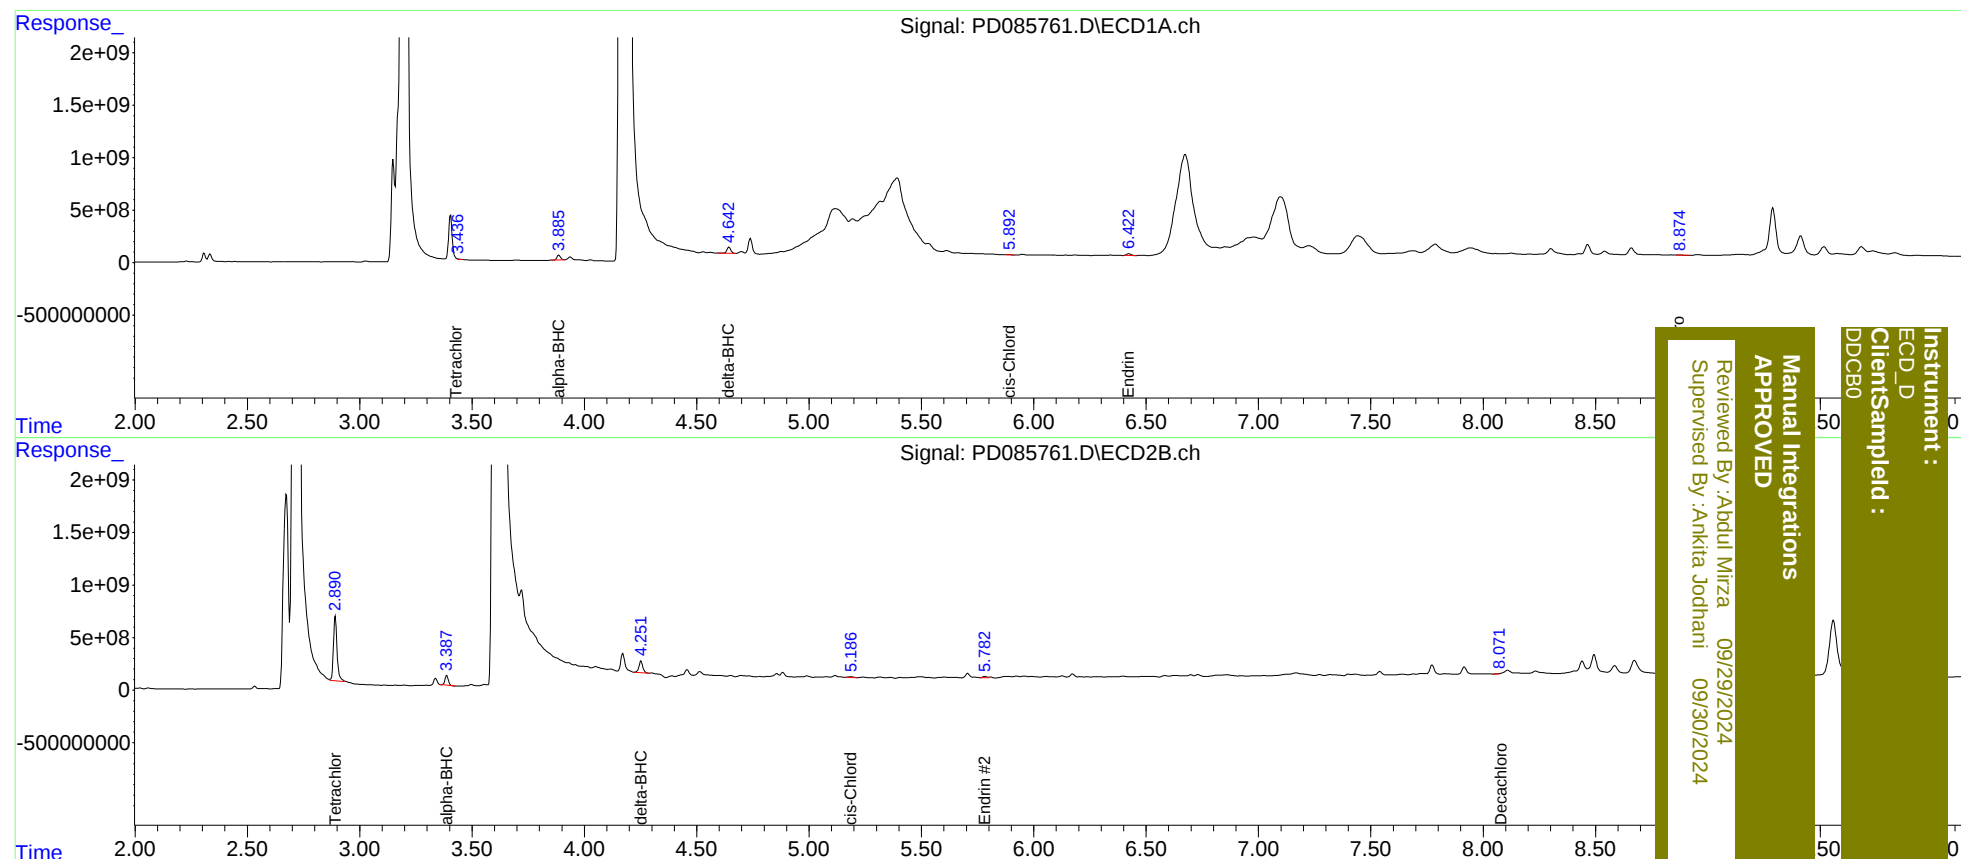

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/29/2024
Supervised By: Ankita Jodhani 09/30/2024

Instrument :
ECD_D
ClientSampled :
DDCB0