

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 16:36
 Operator : AR\AJ
 Sample : P4019-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCFO

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/01/2024
 Supervised By : Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 21:14:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.889	18575229	212.1E6	17.731m	50.104 #
27)	SA Decachlor...	8.893	8.064	26760552	54368360	18.153	14.061
Target Compounds							
2)	A alpha-BHC	3.886	3.388	18064335	64286911	9.926	9.953
3)	MA gamma-BHC...	4.203	3.722	57048931	90275921	30.134m	14.657 #
6)	B beta-BHC	4.398	4.016	3975957	10582331	5.077m	3.957
7)	B delta-BHC	4.648	4.252	28554990	91251818	16.133m	15.305

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 16:36
Operator : AR\AJ
Sample : P4019-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 21:14:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

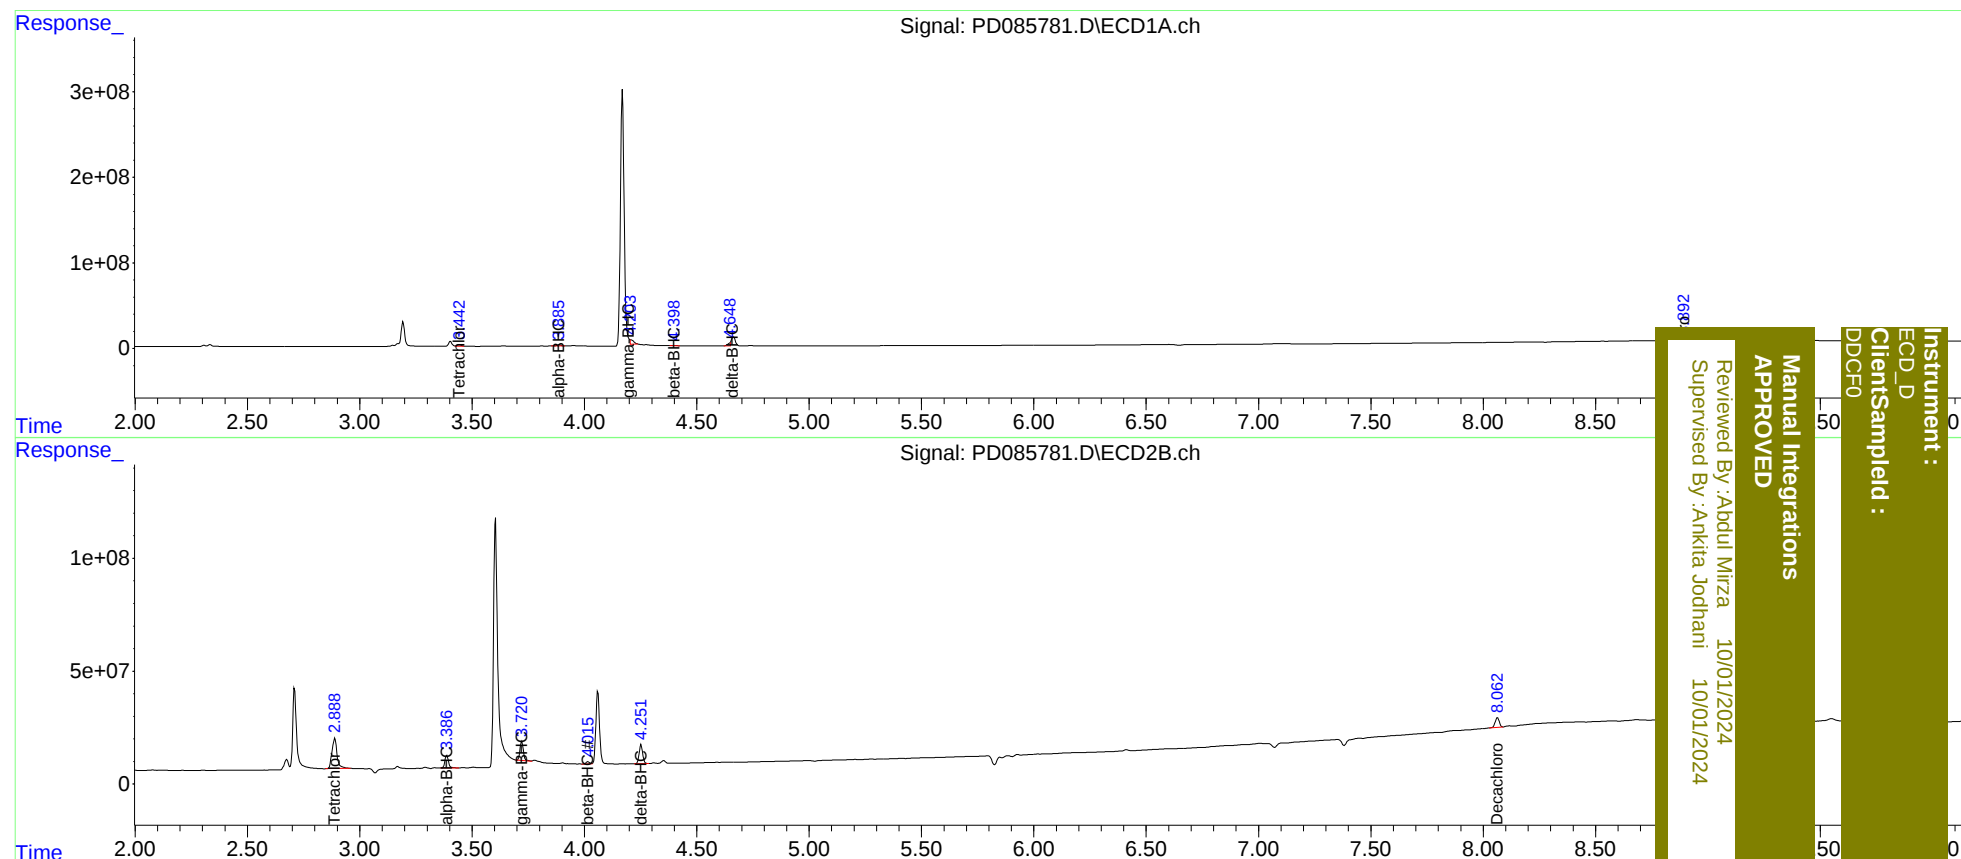

Instrument :
ECD_D
ClientSampled :
DDCF0

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/01/2024
Supervised By : Ankita Jodhani 10/01/2024