

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 18:37
 Operator : AR\AJ
 Sample : P4020-08MSD
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCG0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/01/2024
 Supervised By :Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 21:16:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.890	13874795	175.4E6	13.244m	41.434 #
2)	SA Decachlor...	8.893	8.062	21096990	46862755	14.312	12.120m
Target Compounds							
2)	A alpha-BHC	3.887	3.388	96744139	290.8E6	53.158	45.022
3)	MA gamma-BHC...	4.209	3.722	246.5E6	261.2E6	130.209m	42.403 #
4)	MA Heptachlor	4.806	4.063	92328070	613.1E6	54.001	102.557 #
5)	MB Aldrin	5.145	4.359	96680552	252.7E6	57.487	42.450 #
6)	B beta-BHC	4.397	4.015	34297319	106.6E6	43.792m	39.856
7)	B delta-BHC	4.645	4.252	96066620	275.0E6	54.276m	46.123
8)	B Heptachlo...	5.564	4.862	85181759	236.1E6	54.473	43.056
9)	A Endosulfan I	5.944	5.236	84193987	221.2E6	56.316	43.172
10)	B trans-Chl...	5.818	5.115	84492663	250.5E6	56.615	46.282
11)	B cis-Chlor...	5.898	5.179	86441149	249.6E6	55.431	45.171
12)	B 4,4'-DDE	6.070	5.364	160.2E6	458.0E6	118.036	92.040
13)	MA Dieldrin	6.217	5.503	181.5E6	488.2E6	111.202	86.403
14)	MA Endrin	6.442	5.780	153.0E6	493.8E6	127.436	110.034
15)	B Endosulfa...	6.655	6.072	125.9E6	404.5E6	91.966	88.065
16)	A 4,4'-DDD	6.577	5.920	127.4E6	363.4E6	115.642	85.487 #
17)	MA 4,4'-DDT	6.891	6.174	125.0E6	387.4E6	112.504	88.636
18)	B Endrin al...	6.783	6.250	112.3E6	306.6E6	107.816	87.571
19)	B Endosulfa...	7.017	6.475	140.2E6	382.7E6	108.509	91.327
20)	A Methoxychlor	7.364	6.746	365.7E6	890.9E6	582.809	422.640 #
21)	B Endrin ke...	7.493	6.985	162.6E6	446.0E6	116.191	83.622 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 18:37
Operator : AR\AJ
Sample : P4020-08MSD
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 21:16:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

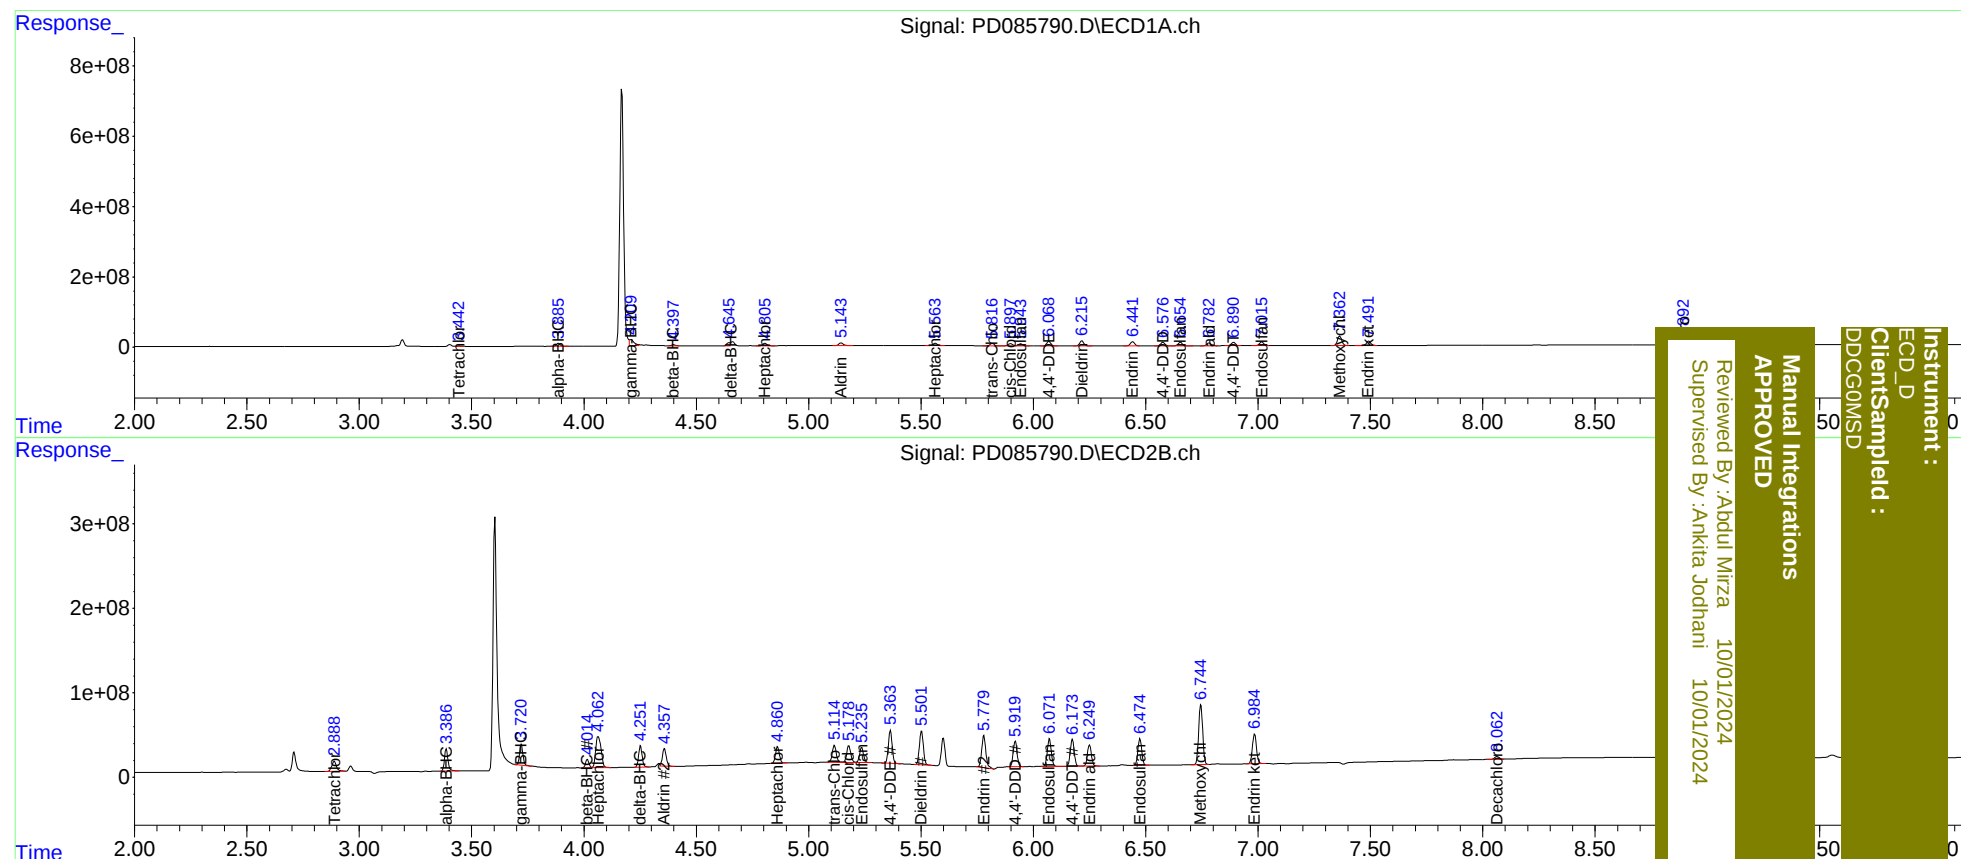

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/01/2024
Supervised By: Ankita Jodhani 10/01/2024

Instrument :
ECD_D
Client Sampled :
DDCGMSD