

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 13:01
 Operator : AR\AJ
 Sample : P4020-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCK4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/01/2024
 Supervised By : Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 13:45:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	2.891	26541850	13590.1E6	25.335m	3209.718 #
27)	SA Decachlor...	8.883	8.048	31665439	7972762	21.481m	2.062m#
Target Compounds							
2)	A alpha-BHC	3.887	3.387	493.7E6	1176.2E6	271.281	182.106 #
7)	B delta-BHC	4.644	4.253	622.3E6	1269.4E6	351.606	212.911 #
8)	B Heptachlo...	5.537	4.858	265.5E6	1003.8E6	169.814	183.036
10)	B trans-Chl...	5.803	5.116	24985219	108.6E6	16.741m	20.064m
11)	B cis-Chlor...	5.893	5.186	35750996	114.1E6	22.925m	20.648
14)	MA Endrin	6.422	5.781	49535824	163.9E6	41.255m	36.519m
17)	MA 4,4'-DDT	6.890	6.172	22162518	188.3E6	19.941m	43.084m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 13:01
Operator : AR\AJ
Sample : P4020-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 13:45:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

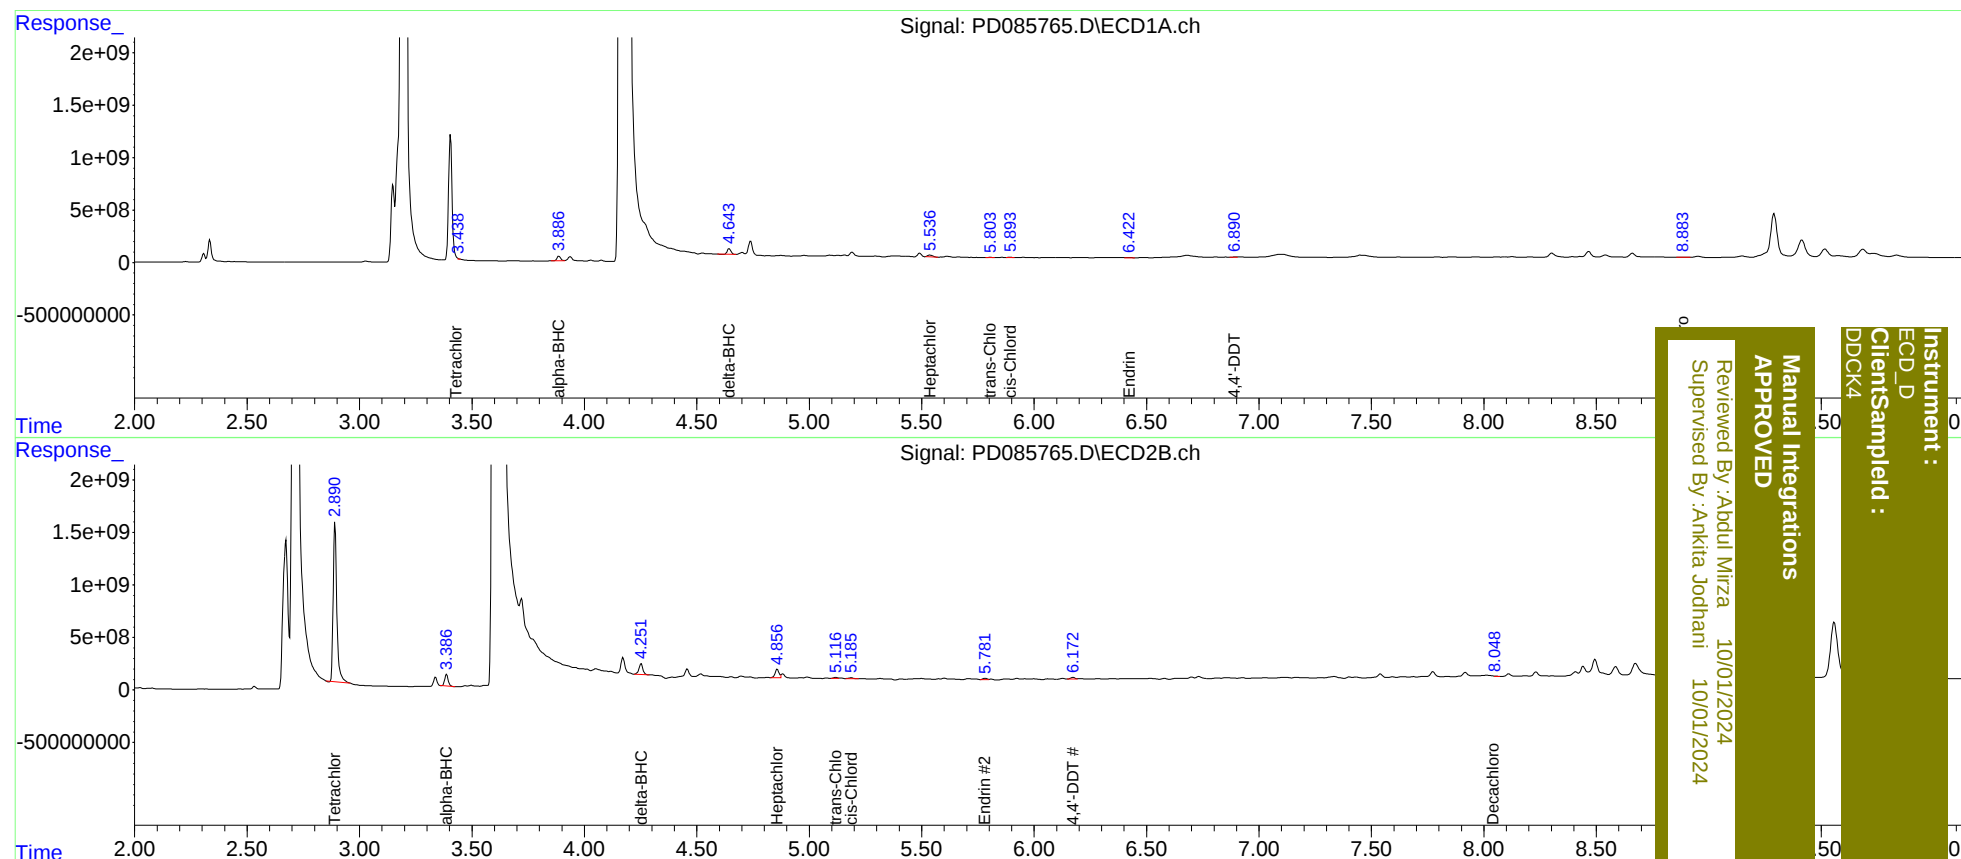

Reviewed By: Abdul Miza 10/01/2024
Supervised By: Ankita Jodhani 10/01/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDCK4