

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 14:22
 Operator : AR\AJ
 Sample : P4021-03MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCG1MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/01/2024
 Supervised By :Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 21:12:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.890	22053176	1079.5E6	21.050m	254.950 #
27)	SA Decachlor...	8.892	8.063	20926213	48385434	14.196m	12.514m
Target Compounds							
2)	A alpha-BHC	3.887	3.387	108.4E6	289.3E6	59.568	44.798
3)	MA gamma-BHC...	4.203	3.720	170.8E6	239.5E6	90.242m	38.879m#
4)	MA Heptachlor	4.807	4.067	95501731	512.5E6	55.858	85.722 #
5)	MB Aldrin	5.146	4.358	101.5E6	259.5E6	60.348	43.598 #
6)	B beta-BHC	4.398	4.015	35829605	105.8E6	45.748m	39.554
7)	B delta-BHC	4.644	4.252	115.6E6	290.1E6	65.328m	48.654 #
8)	B Heptachlo...	5.564	4.862	87875344	243.7E6	56.195	44.442
9)	A Endosulfan I	5.945	5.236	87077956	232.4E6	58.245	45.357
10)	B trans-Chl...	5.818	5.115	94750019	250.7E6	63.488	46.304 #
11)	B cis-Chlor...	5.899	5.179	90864614	252.2E6	58.267	45.628
12)	B 4,4'-DDE	6.070	5.364	171.7E6	473.0E6	126.529	95.069
13)	MA Dieldrin	6.217	5.503	191.1E6	505.2E6	117.062	89.412
14)	MA Endrin	6.442	5.780	163.6E6	540.8E6	136.277	120.494
15)	B Endosulfa...	6.655	6.072	129.0E6	410.6E6	94.225	89.403
16)	A 4,4'-DDD	6.577	5.920	135.3E6	381.3E6	122.770	89.698 #
17)	MA 4,4'-DDT	6.892	6.174	133.8E6	399.0E6	120.410	91.279
18)	B Endrin al...	6.783	6.251	116.6E6	307.5E6	111.927	87.815
19)	B Endosulfa...	7.017	6.475	145.2E6	386.2E6	112.410	92.154
20)	A Methoxychlor	7.364	6.747	379.3E6	899.7E6	604.448	426.845 #
21)	B Endrin ke...	7.494	6.985	177.1E6	441.7E6	126.541	82.813 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 14:22
Operator : AR\AJ
Sample : P4021-03MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 21:12:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

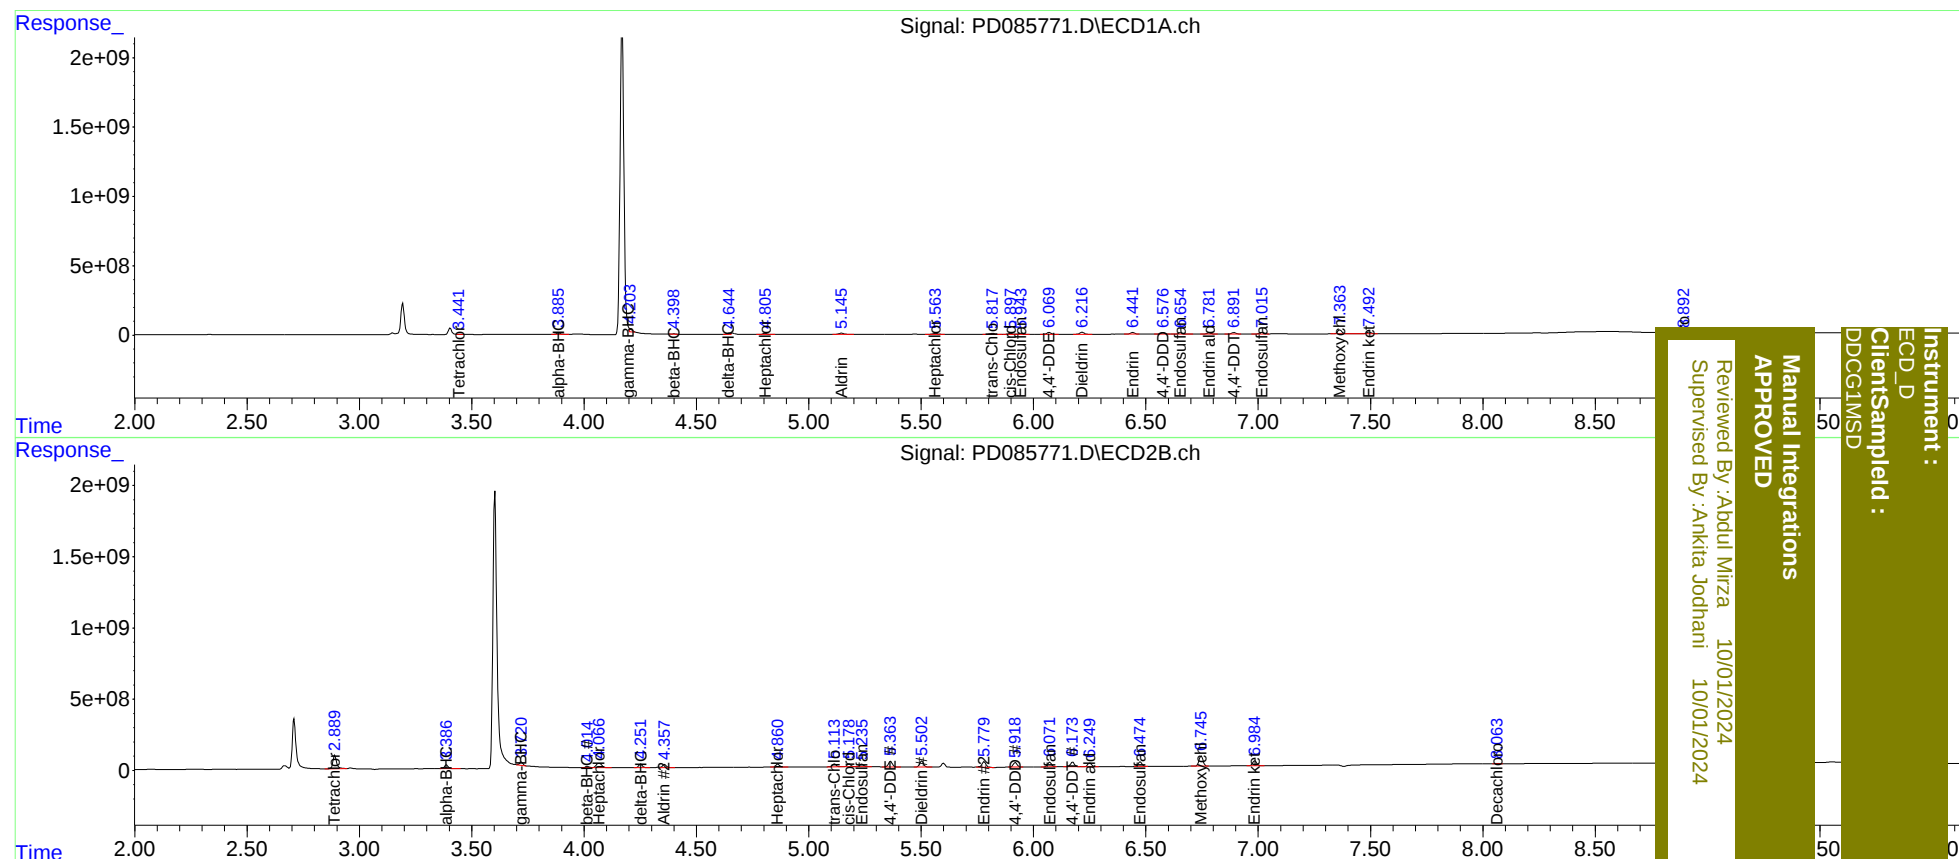

Instrument :
ECD_D
Client Sampled :
DDCG1MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/01/2024
Supervised By: Ankita Jodhani 10/01/2024