

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
 Data File : PD085784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2024 17:17
 Operator : AR\AJ
 Sample : P4019-19
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCF3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/29/2024
 Supervised By : Ankita Jodhani 09/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 21:15:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	2.879	11166436	58328831	10.659m	13.776 #
2) SA Decachlor...	8.892	8.064	18281113	37101459	12.401m	9.596
Target Compounds						
3) MA gamma-BHC...	4.199	3.721	4401710	6193366	2.325m	1.006 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092824\
Data File : PD085784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2024 17:17
Operator : AR\AJ
Sample : P4019-19
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 21:15:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

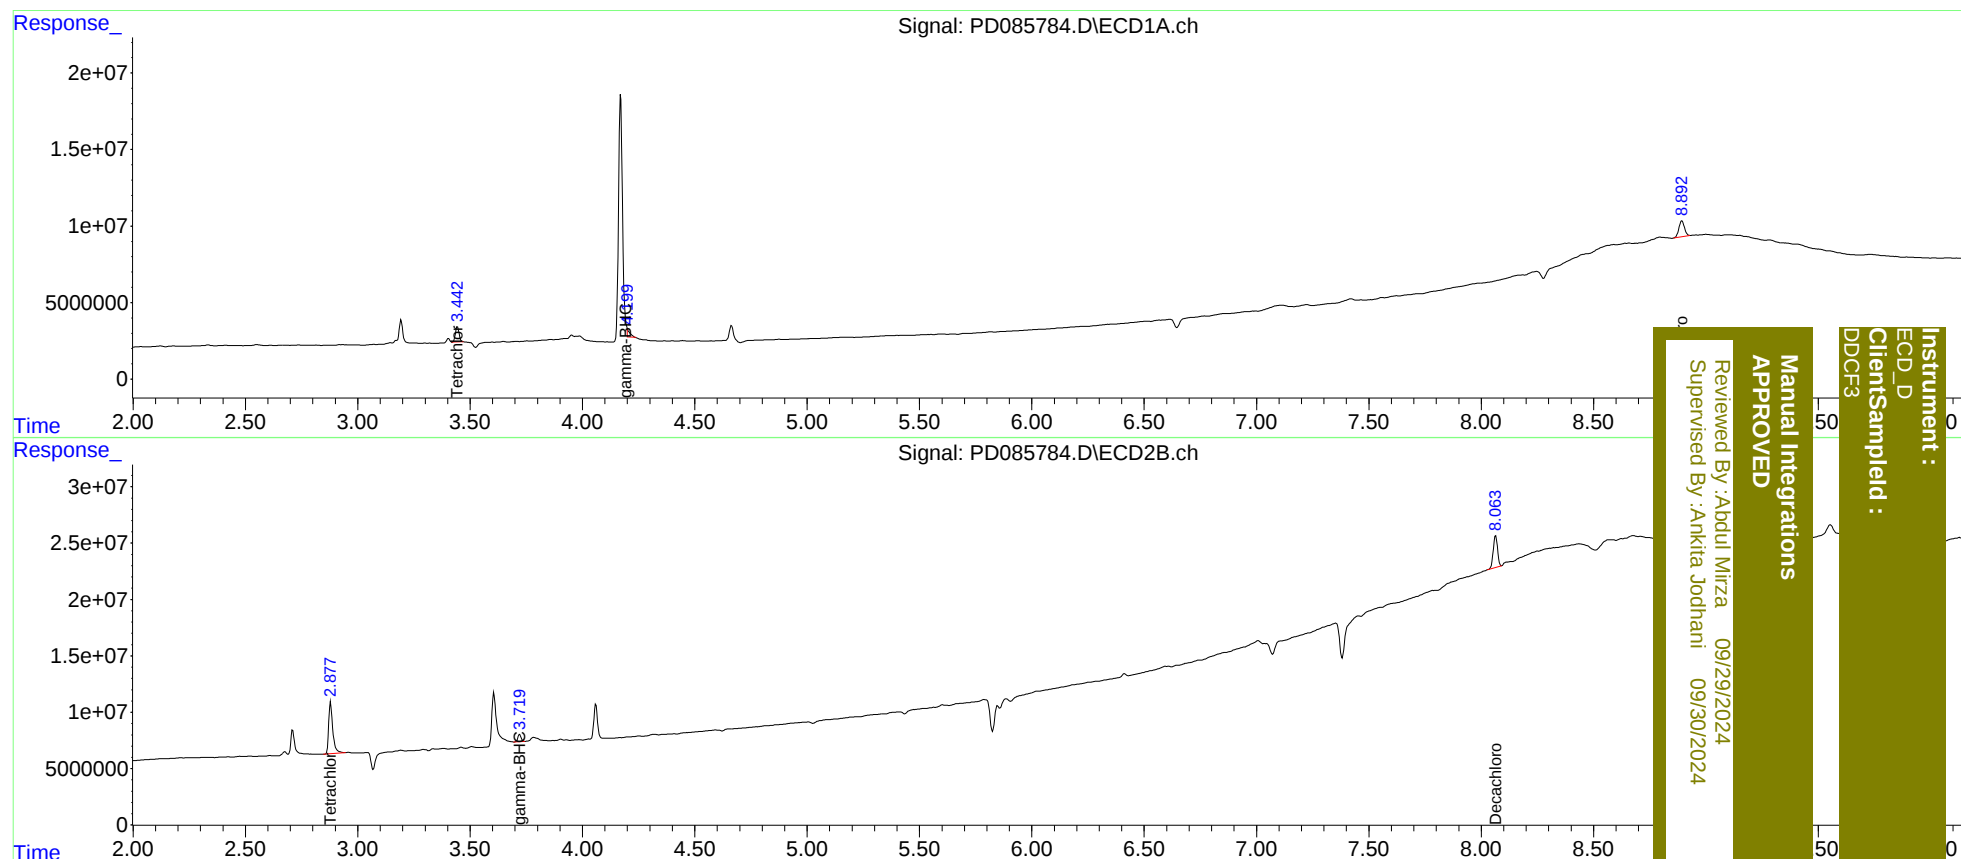

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/29/2024
Supervised By: Ankita Jodhani 09/30/2024

Instrument :
ECD_D
ClientSampled :
DDCF3