

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
 Data File : PD065961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2021 11:26
 Operator : AR\AJ
 Sample : PB139385BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS385

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:49:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	17633850	138.4E6	20.374	19.458
27)	SA Decachlor...	8.235	9.086	50934615	157.9E6	34.446	36.508
Target Compounds							
2)	A alpha-BHC	3.932	4.407	4826808	38571897	4.080	4.057
3)	MA gamma-BHC...	4.215	4.693	5701127	40208454	4.664	4.399
4)	MA Heptachlor	4.513	5.197	6147551	51940279	4.812	6.173 #
5)	MB Aldrin	4.760	5.502	6295150	40186801	5.064	4.996
6)	B beta-BHC	4.464	4.869	3120685	23009255	4.724	5.115
7)	B delta-BHC	4.668	5.086	535790	4872470	0.429	0.537 #
8)	B Heptachlo...	5.203	5.891	6684208	35495880	5.371	5.191
9)	A Endosulfan I	5.541	6.250	6445201	33133844	5.400	5.078
10)	B trans-Chl...	5.428	6.126	7056272	35462564	5.416	4.976
11)	B cis-Chlor...	5.486	6.197	6961995	35192789	5.351	5.038
12)	B 4,4'-DDE	5.649	6.356	12190414	68490222	10.227	10.511
13)	MA Dieldrin	5.784	6.508	13165669	69951940	10.174	10.243
14)	MA Endrin	6.042	6.727	9544032	45365258	8.117	8.131
15)	B Endosulfa...	6.314	6.941	13101684	59487749	10.493	9.992
16)	A 4,4'-DDD	6.164	6.851	10774555	56936464	10.076	10.309
17)	MA 4,4'-DDT	6.404	7.148	10419585	47772226	8.985	8.830
18)	B Endrin al...	6.483	7.066	12207981	53748799	12.347	11.543
19)	B Endosulfa...	6.695	7.288	9767712	39477281	7.681	6.991
20)	A Methoxychlor	6.951	7.608	33563474	125.9E6	48.798	48.221
21)	B Endrin ke...	7.189	7.762	17563641	68714907	11.521	10.691

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
Data File : PD065961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2021 11:26
Operator : AR\AJ
Sample : PB139385BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:49:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

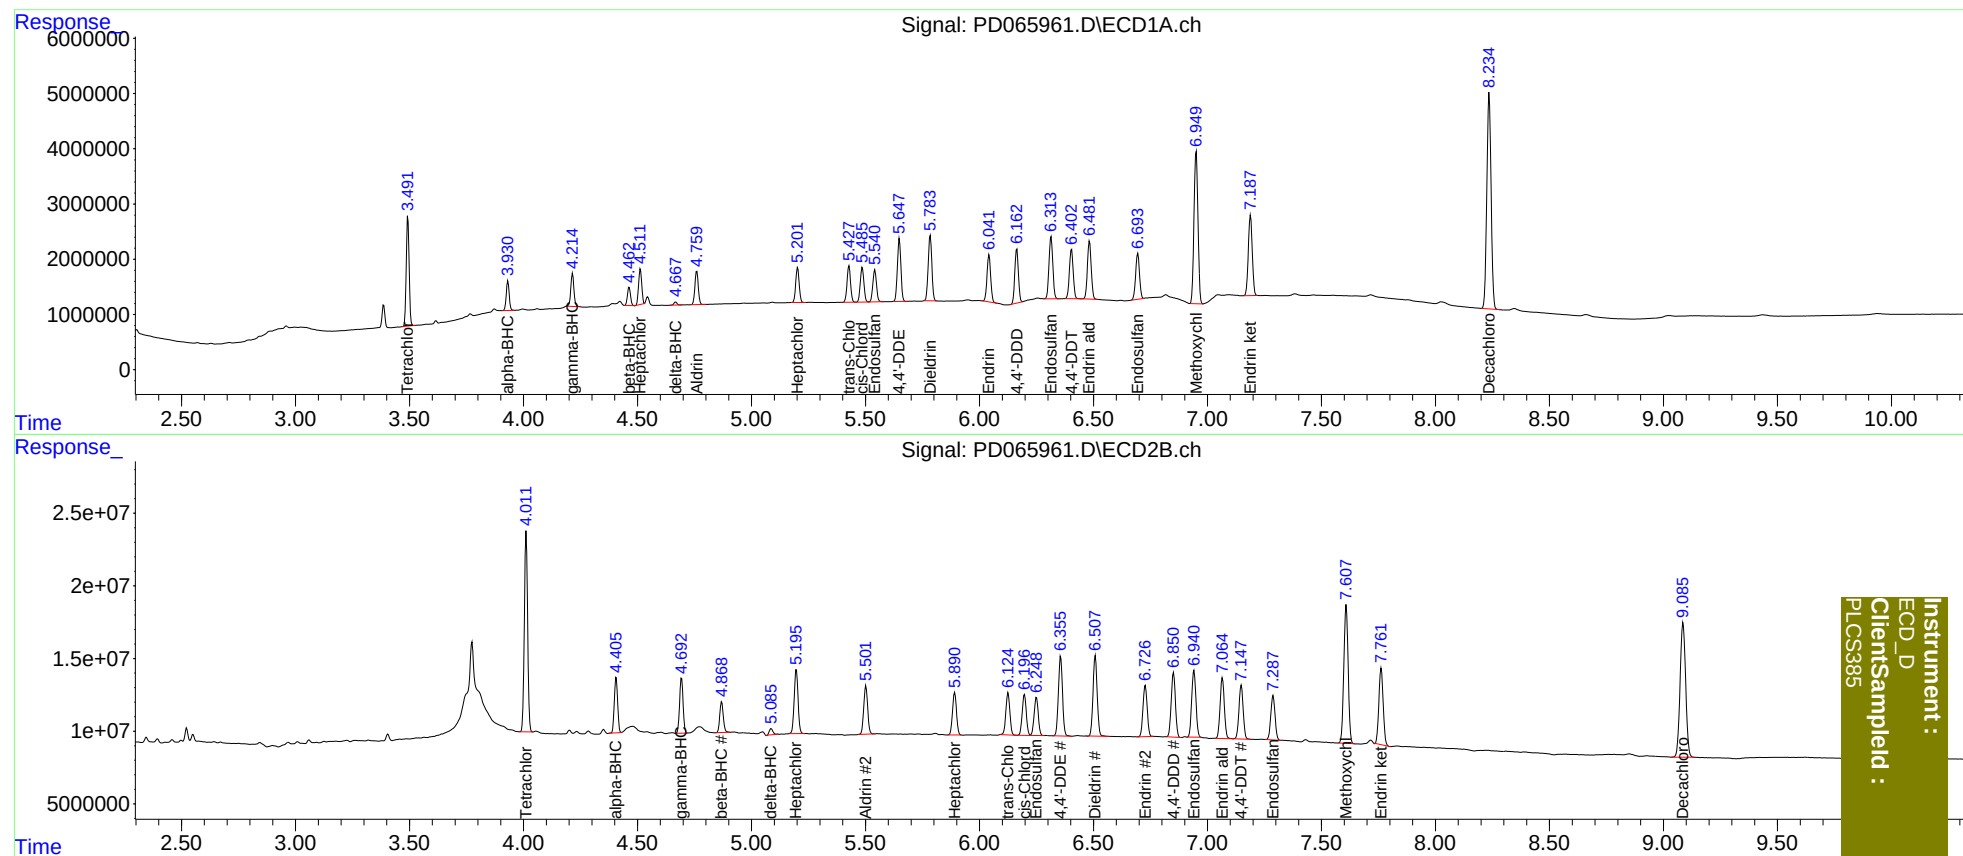

Instrument :
ECD_D
ClientSampled :
PLCS385