

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
 Data File : PD065971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2021 17:00
 Operator : AR\AJ
 Sample : M3878-16MSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2N4MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:52:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	19034294	142.2E6	21.992	20.000
2)	SA Decachlor...	8.235	9.085	53036825	160.6E6	35.868	37.140
Target Compounds							
2)	A alpha-BHC	3.932	4.407	72355411	475.2E6	61.166	49.980
3)	MA gamma-BHC...	4.215	4.693	71041997	443.2E6	58.118	48.495
4)	MA Heptachlor	4.513	5.197	72317274	386.2E6	56.604	45.895
5)	MB Aldrin	4.760	5.502	69393611	359.8E6	55.826	44.729
6)	B beta-BHC	4.463	4.870	31971214	199.7E6	48.398	44.390
7)	B delta-BHC	4.668	5.086	72053682	431.3E6	57.648	47.555
8)	B Heptachlo...	5.203	5.892	70647497	331.1E6	56.768	48.417
9)	A Endosulfan I	5.541	6.250	67827724	314.9E6	56.832	48.268
10)	B trans-Chl...	5.427	6.126	73560179	334.3E6	56.463	46.903
11)	B cis-Chlor...	5.486	6.197	72592483	328.1E6	55.793	46.968
12)	B 4,4'-DDE	5.648	6.356	143.4E6	637.9E6	120.274	97.900
13)	MA Dieldrin	5.784	6.508	154.3E6	670.6E6	119.246	98.194
14)	MA Endrin	6.041	6.727	123.2E6	507.4E6	104.800	90.952
15)	B Endosulfa...	6.314	6.940	134.9E6	560.3E6	108.059	94.114
16)	A 4,4'-DDD	6.164	6.850	128.8E6	547.7E6	120.410	99.174
17)	MA 4,4'-DDT	6.403	7.148	133.7E6	518.3E6	115.317	95.799
18)	B Endrin al...	6.482	7.065	116.6E6	476.6E6	117.883	102.361
19)	B Endosulfa...	6.694	7.288	136.4E6	531.8E6	107.278	94.175
20)	A Methoxychlor	6.950	7.608	362.5E6	1181.7E6	527.068	452.523
21)	B Endrin ke...	7.188	7.761	175.7E6	618.9E6	115.229	96.293

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
Data File : PD065971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2021 17:00
Operator : AR\AJ
Sample : M3878-16MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:52:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

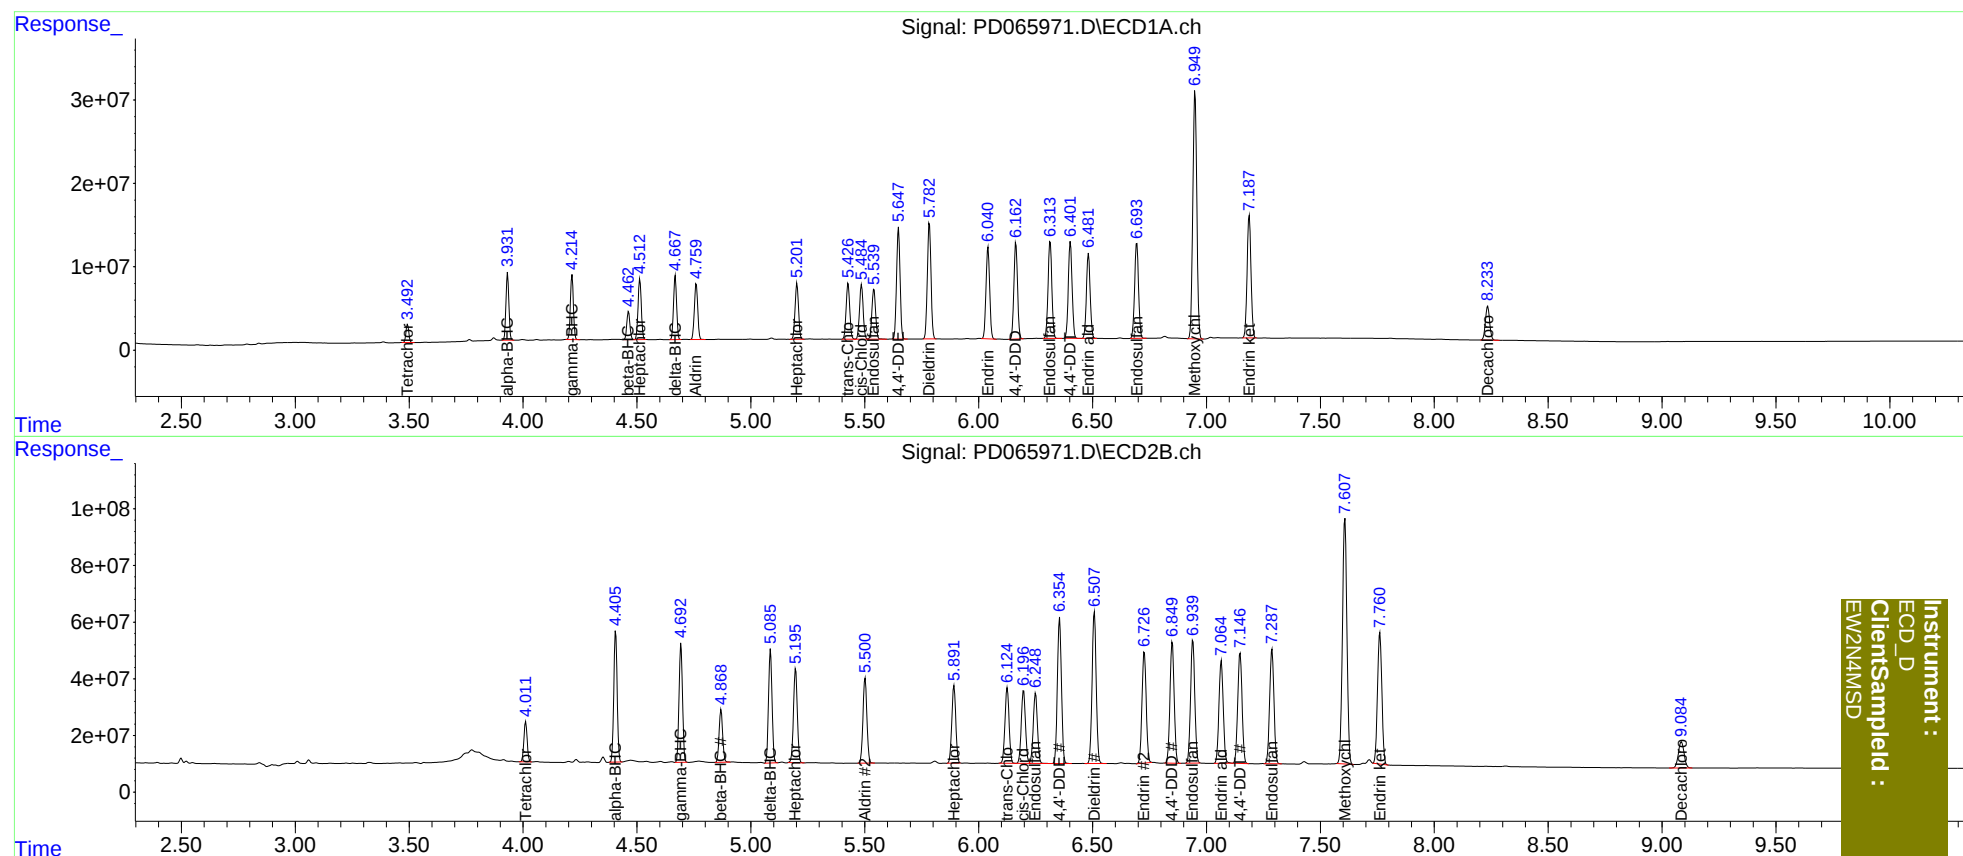

Instrument :
ECD_D
ClientSampled :
EW2N4MSD