

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
 Data File : PD065970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2021 16:46
 Operator : AR\AJ
 Sample : M3878-15MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2N4MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:52:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	19665871	146.2E6	22.722	20.560
27)	SA Decachlor...	8.235	9.085	47089232	143.6E6	31.845	33.201
Target Compounds							
2)	A alpha-BHC	3.932	4.407	73750164	482.1E6	62.345	50.710
3)	MA gamma-BHC...	4.216	4.694	72180805	447.1E6	59.050	48.922
4)	MA Heptachlor	4.513	5.197	72801633	388.0E6	56.983	46.112
5)	MB Aldrin	4.761	5.502	69743042	359.3E6	56.107	44.667
6)	B beta-BHC	4.464	4.870	32395468	201.4E6	49.040	44.768
7)	B delta-BHC	4.669	5.086	73337679	434.1E6	58.676	47.854
8)	B Heptachlo...	5.203	5.892	71608060	334.5E6	57.540	48.921
9)	A Endosulfan I	5.541	6.250	68408427	317.5E6	57.318	48.662
10)	B trans-Chl...	5.428	6.126	74342654	338.2E6	57.064	47.447
11)	B cis-Chlor...	5.486	6.197	73410869	331.5E6	56.422	47.460
12)	B 4,4'-DDE	5.649	6.356	145.3E6	644.0E6	121.864	98.830
13)	MA Dieldrin	5.784	6.508	156.5E6	680.1E6	120.902	99.581
14)	MA Endrin	6.042	6.728	125.5E6	498.2E6	106.703	89.291
15)	B Endosulfa...	6.314	6.941	137.8E6	568.4E6	110.378	95.468
16)	A 4,4'-DDD	6.164	6.851	129.9E6	555.1E6	121.511	100.502
17)	MA 4,4'-DDT	6.404	7.148	136.0E6	525.6E6	117.298	97.151
18)	B Endrin al...	6.483	7.066	118.2E6	483.1E6	119.512	103.758
19)	B Endosulfa...	6.695	7.288	139.2E6	539.8E6	109.457	95.587
20)	A Methoxychlor	6.950	7.608	367.4E6	1197.8E6	534.228	458.694
21)	B Endrin ke...	7.189	7.761	177.7E6	625.8E6	116.556	97.371

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092921\
Data File : PD065970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2021 16:46
Operator : AR\AJ
Sample : M3878-15MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:52:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

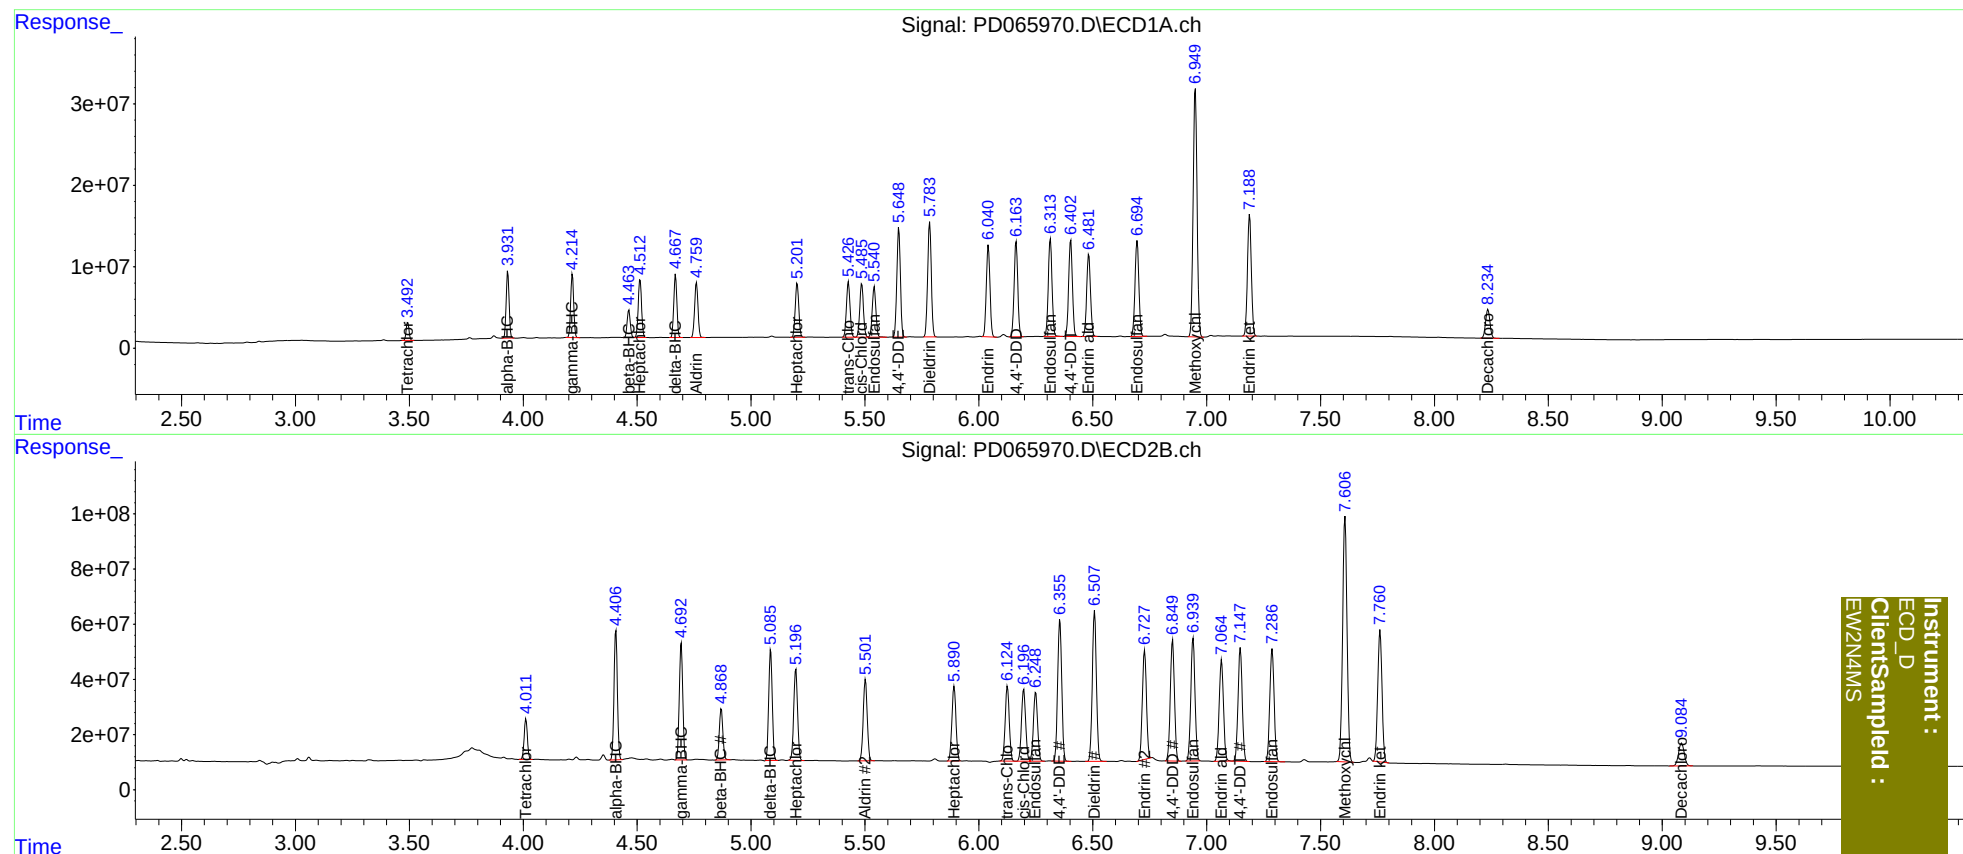

Instrument :
ECD_D
ClientSampled :
EW2N4MS