

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 08:57
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:15:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.721f	0	109686	N.D.	<MDL
Target Compounds						
3) MA gamma-BHC...	0.000	3.605	0	31842	N.D.	<MDL
4) MA Heptachlor	0.000	3.974f	0	169349	N.D.	<MDL
5) MB Aldrin	0.000	4.194	0	3333299	N.D.	1.359
6) B beta-BHC	0.000	3.842f	0	424957	N.D.	0.390
7) B delta-BHC	0.000	4.067f	0	41443	N.D.	<MDL
8) B Heptachlo...	5.694	0.000	6654169	0	1.796	N.D. #
9) A Endosulfan I	0.000	5.047	0	1373600	N.D.	0.668
10) B trans-Chl...	0.000	5.008f	0	1473672	N.D.	0.661
11) B cis-Chlor...	0.000	5.028	0	752957	N.D.	0.328
12) B 4,4'-DDE	0.000	5.166f	0	160396	N.D.	<MDL
14) MA Endrin	0.000	5.601	0	171297	N.D.	<MDL
22) Toxaphene-1	0.000	5.008	0	1473672	N.D.	122.013
23) Toxaphene-2	0.000	5.662	0	78539	N.D.	5.873


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 08:57
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:15:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

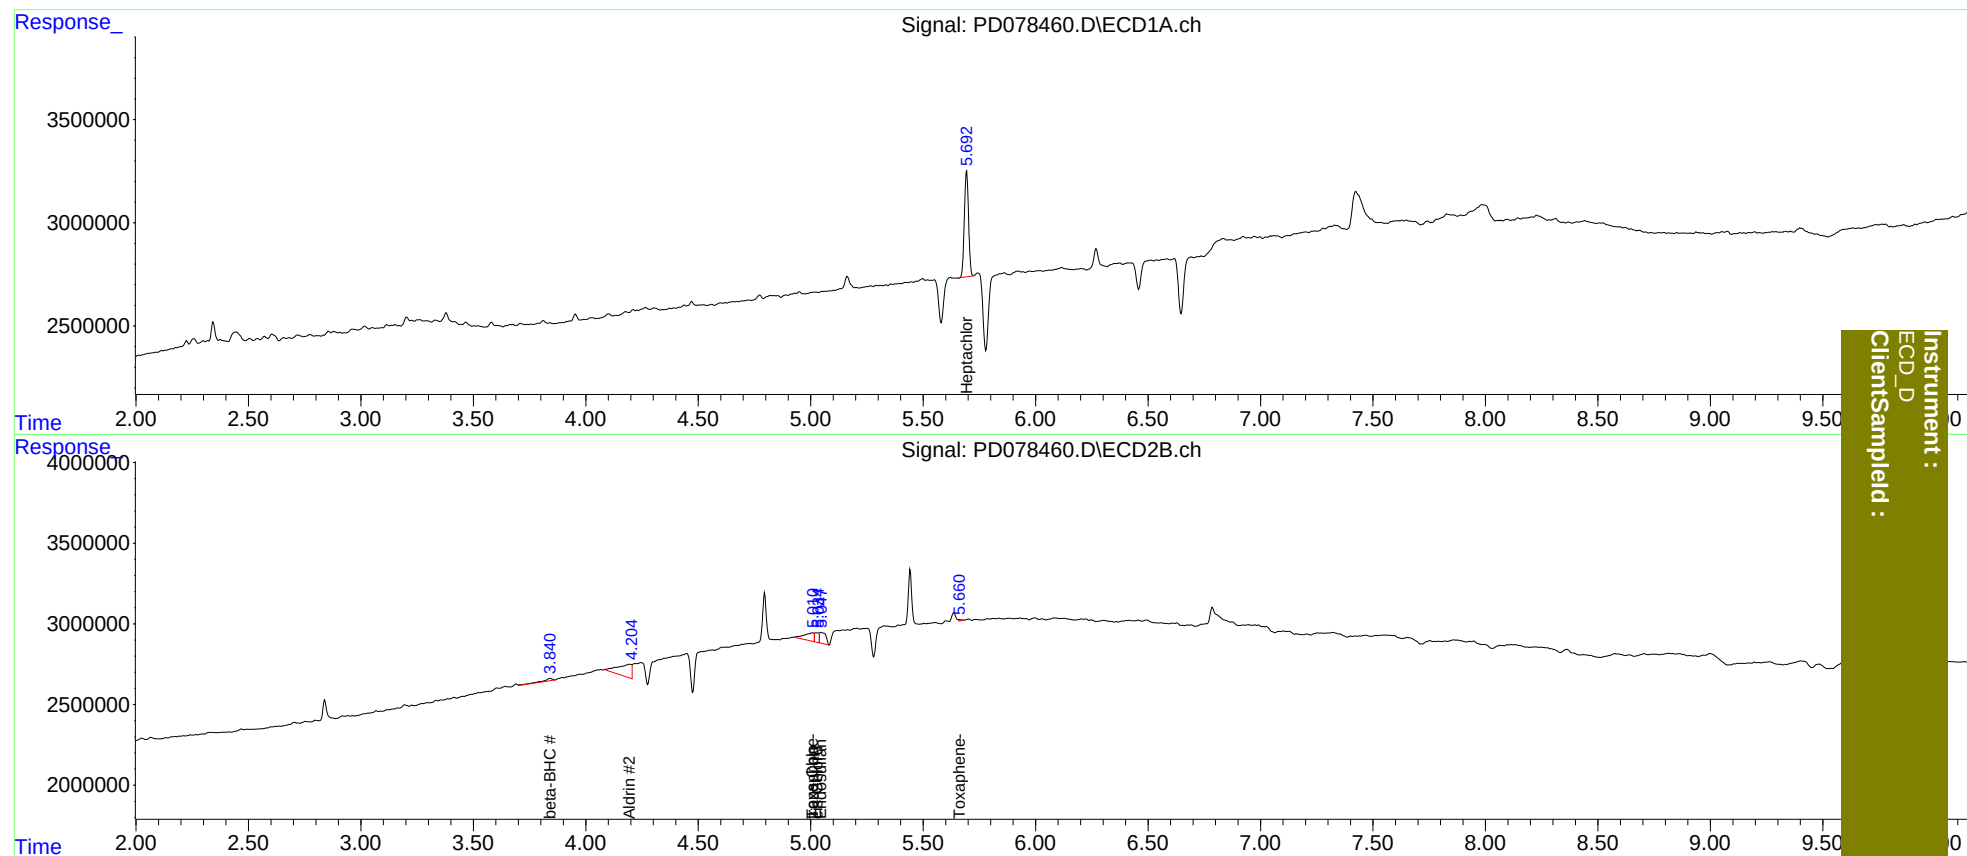


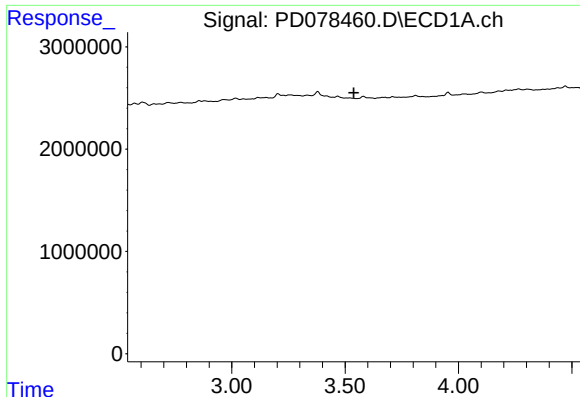

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

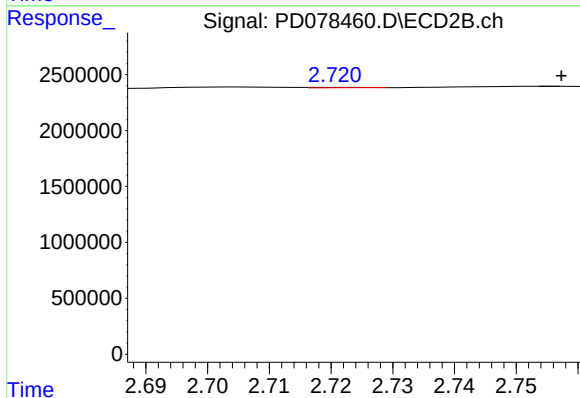

#1 Tetrachloro-m-xylene


R.T.: 2.721 min
Delta R.T.: -0.036 min
Response: 109686
Conc: N.D.

#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

#5 Aldrin


R.T.: 4.194 min
Delta R.T.: -0.012 min
Response: 3333299
Conc: 1.36 ng/ml

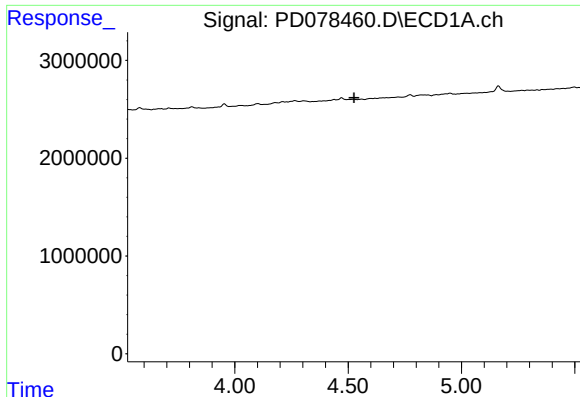

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

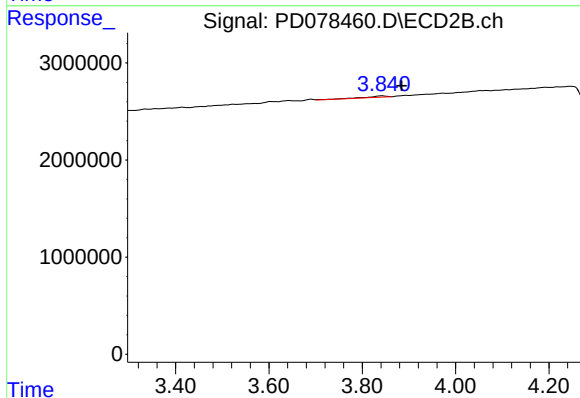


#6 beta-BHC

R.T.: 3.842 min
Delta R.T.: -0.043 min
Response: 424957
Conc: 0.39 ng/ml

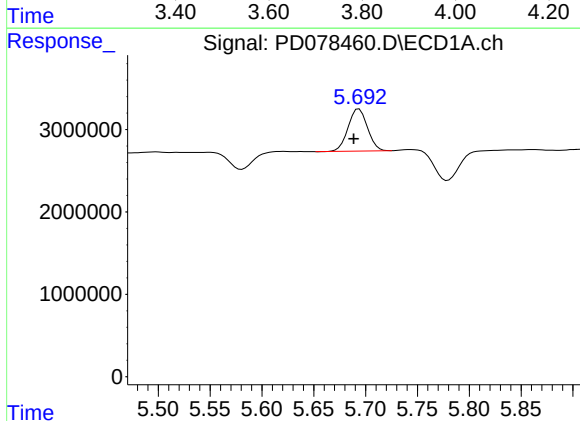


#8 Heptachlor epoxide

R.T.: 5.694 min
Delta R.T.: 0.005 min
Response: 6654169
Conc: 1.80 ng/ml

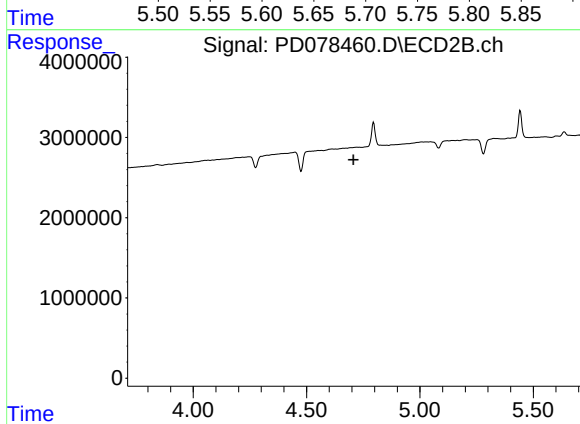

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.708 min
Response: 0
Conc: N.D.

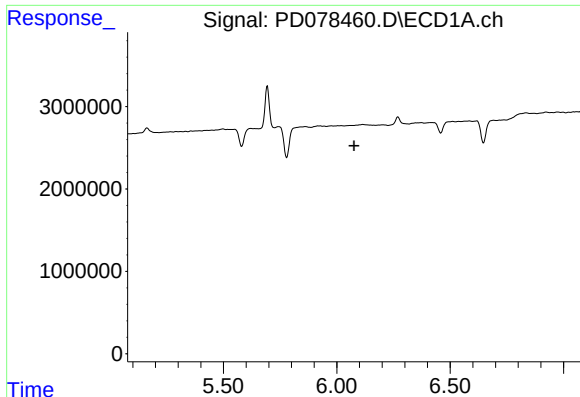

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

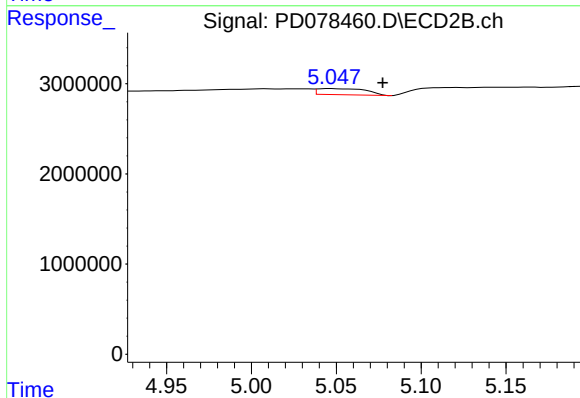


#9 Endosulfan I

R.T.: 5.047 min
Delta R.T.: -0.031 min
Response: 1373600
Conc: 0.67 ng/ml

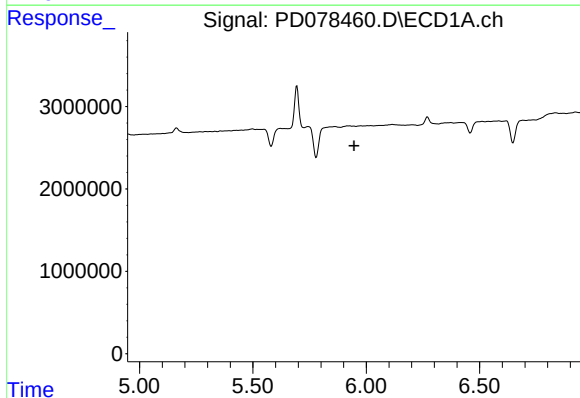


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

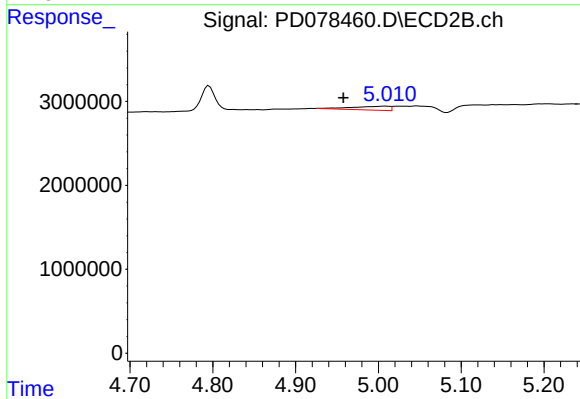

#10 trans-Chlordane


R.T.: 5.008 min
Delta R.T.: 0.050 min
Response: 1473672
Conc: 0.66 ng/ml

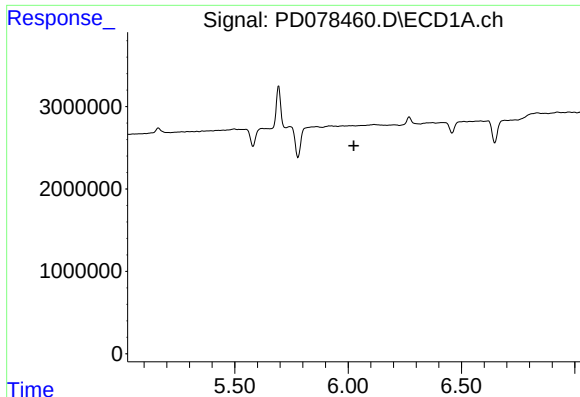

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

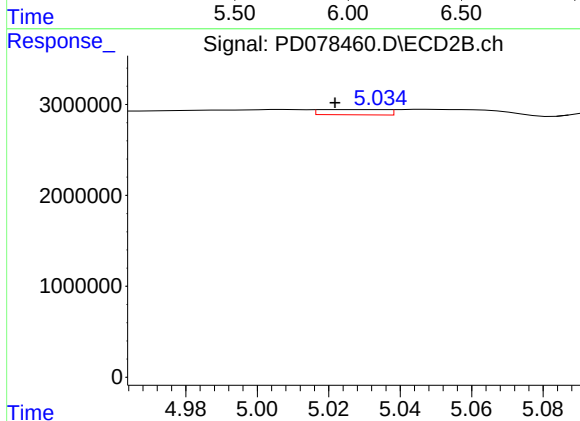


#11 cis-Chlordane

R.T.: 5.028 min
Delta R.T.: 0.006 min
Response: 752957
Conc: 0.33 ng/ml

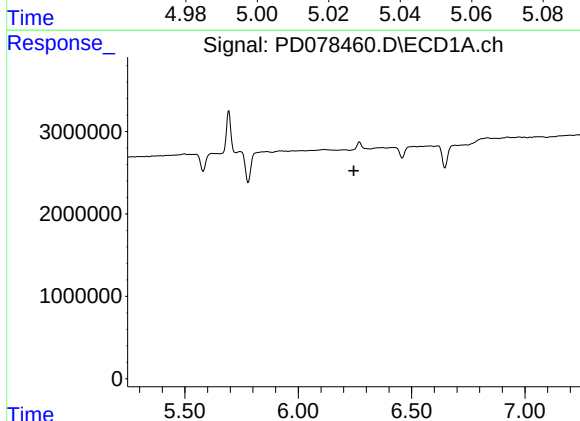


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 6.245 min
Response: 0
Conc: N.D.

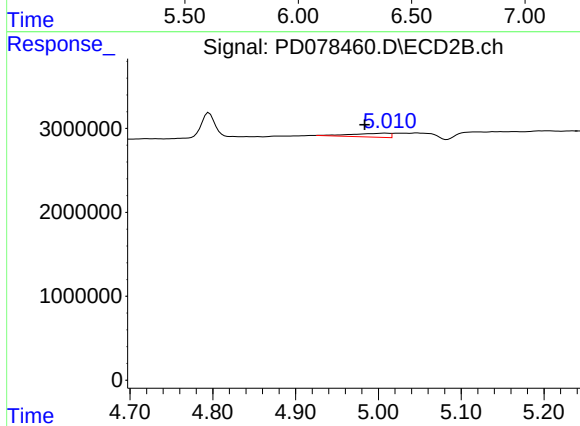

#22 Toxaphene-1


R.T.: 5.008 min
Delta R.T.: 0.024 min
Response: 1473672
Conc: 122.01 ng/ml

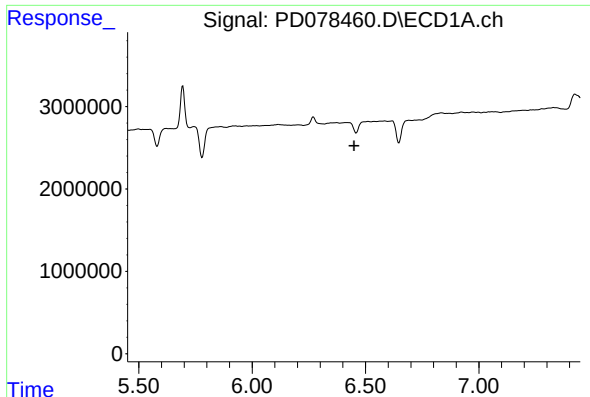

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

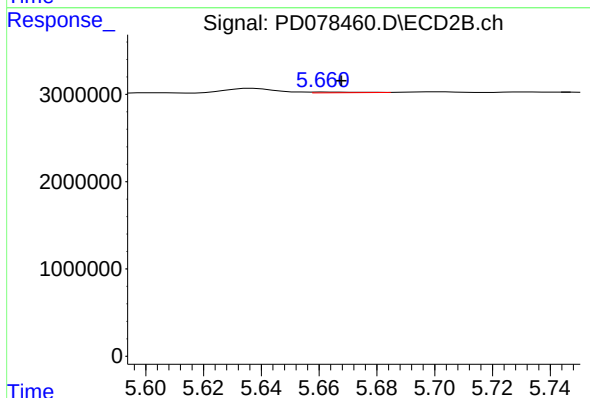


#23 Toxaphene-2

R.T.: 5.662 min
Delta R.T.: -0.006 min
Response: 78539
Conc: 5.87 ng/ml

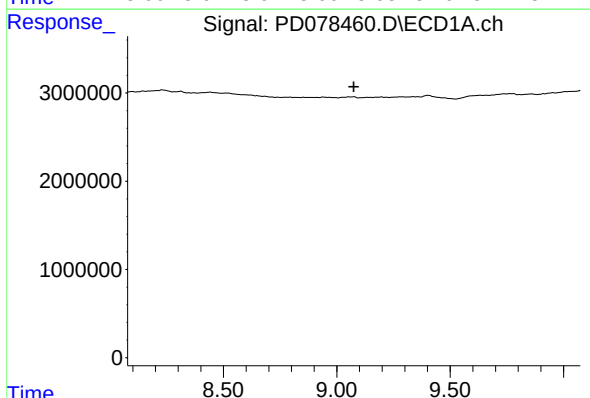

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.076 min
Response: 0
Conc: N.D.

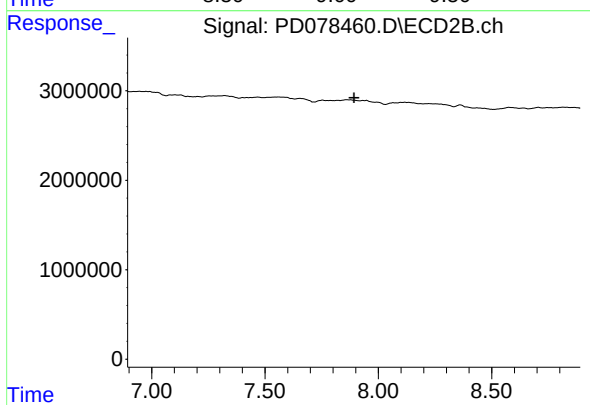

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.893 min
Response: 0
Conc: N.D.