

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 12:48
 Operator : AR\AJ
 Sample : 04607-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:22:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	48797832	33171872	19.873	20.080
27)	SA Decachlor...	9.077	7.893	54720233	30267046	16.928	16.349
Target Compounds							
3)	MA gamma-BHC...	4.295f	0.000	3453631	0	0.871	N.D. #
6)	B beta-BHC	0.000	3.842f	0	455393	N.D.	0.418
9)	A Endosulfan I	0.000	5.120f	0	530586	N.D.	0.258
12)	B 4,4'-DDE	0.000	5.150f	0	231958	N.D.	0.108
21)	B Endrin ke...	0.000	6.867f	0	136727	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 12:48
Operator : AR\AJ
Sample : 04607-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:22:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

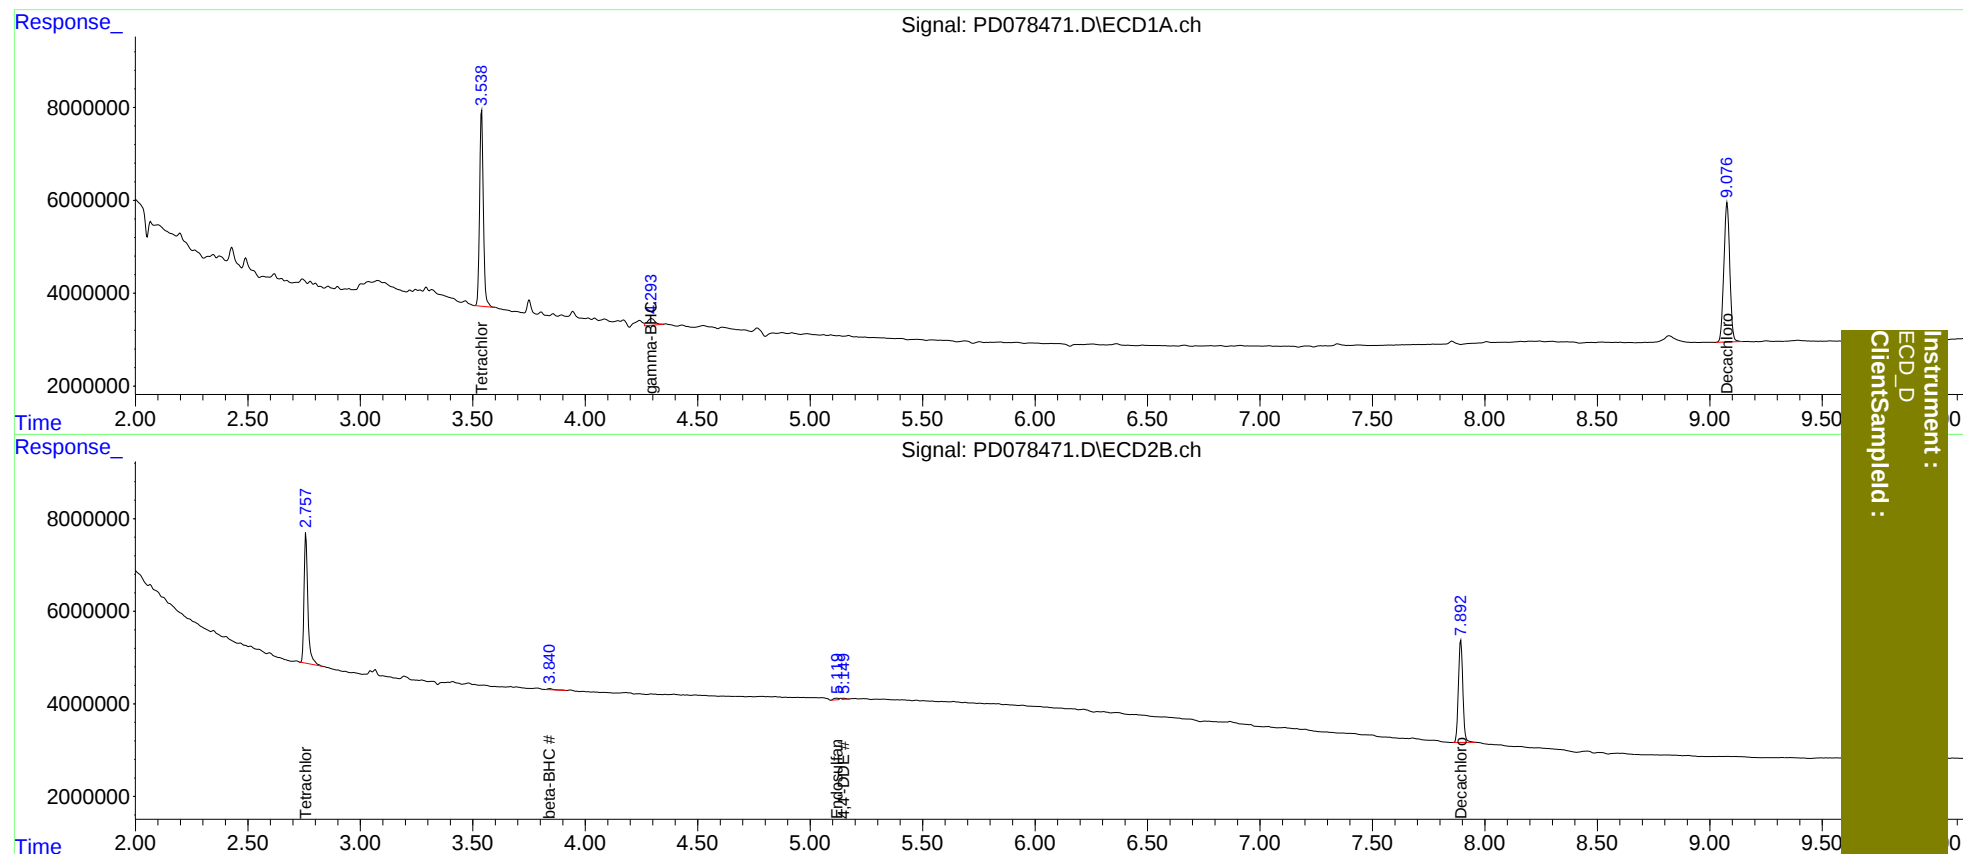


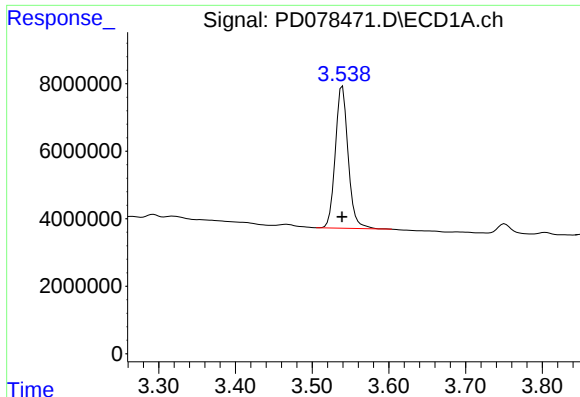

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 48797832
Conc: 19.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

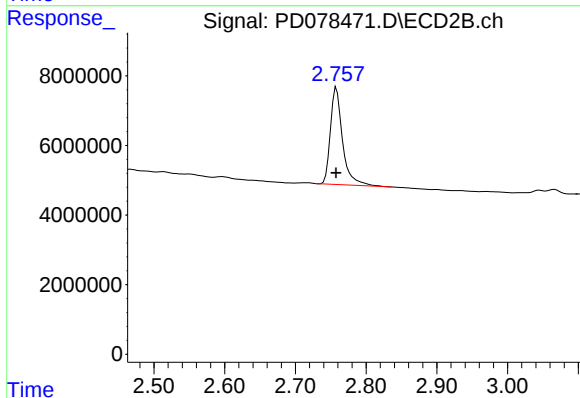


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 33171872
Conc: 20.08 ng/ml

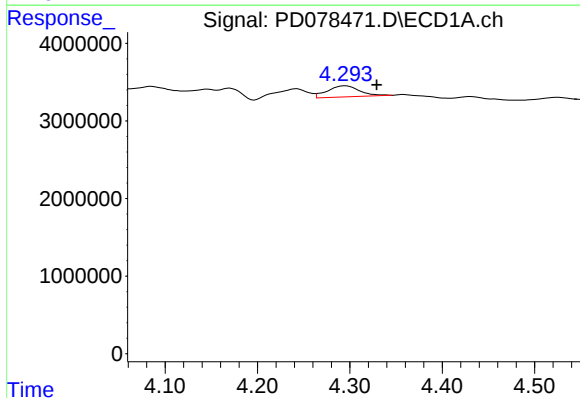


#3 gamma-BHC (Lindane)

R.T.: 4.295 min
Delta R.T.: -0.034 min
Response: 3453631
Conc: 0.87 ng/ml

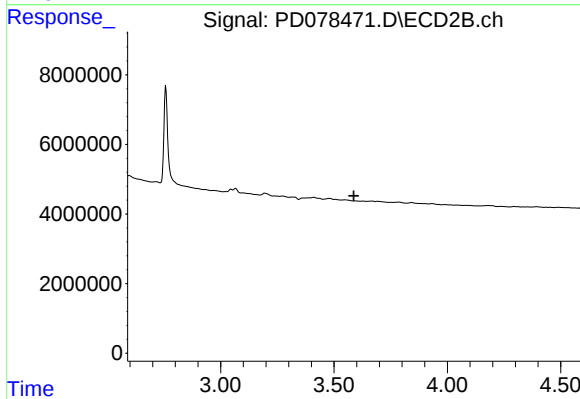

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.588 min
Response: 0
Conc: N.D.

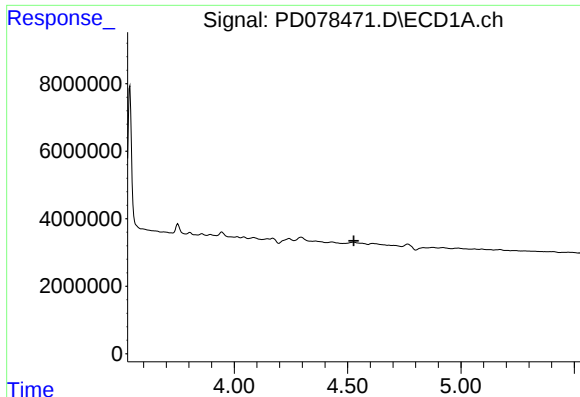

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

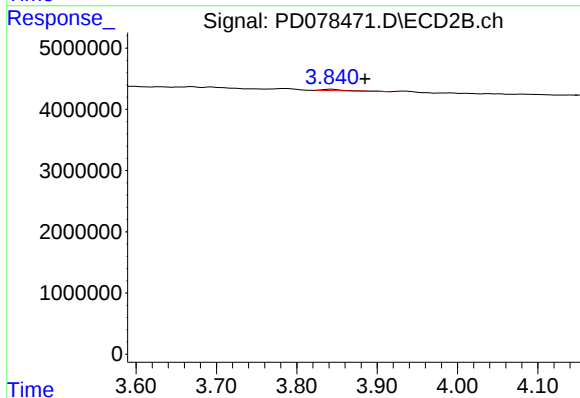


#6 beta-BHC

R.T.: 3.842 min
Delta R.T.: -0.042 min
Response: 455393
Conc: 0.42 ng/ml

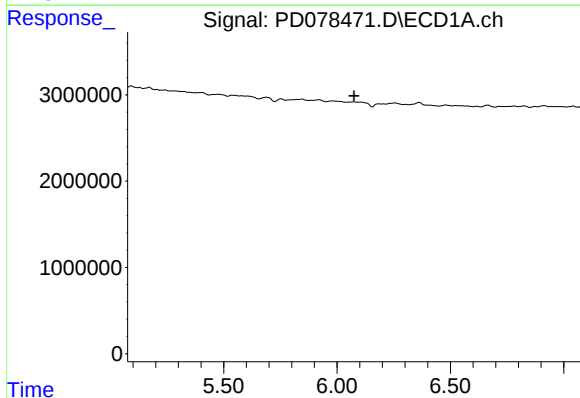


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

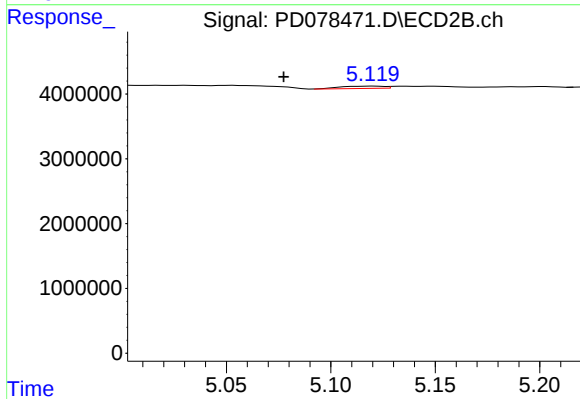

#9 Endosulfan I


R.T.: 5.120 min
Delta R.T.: 0.042 min
Response: 530586
Conc: 0.26 ng/ml

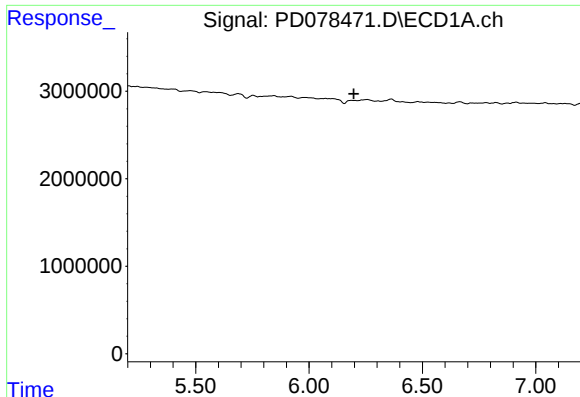

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

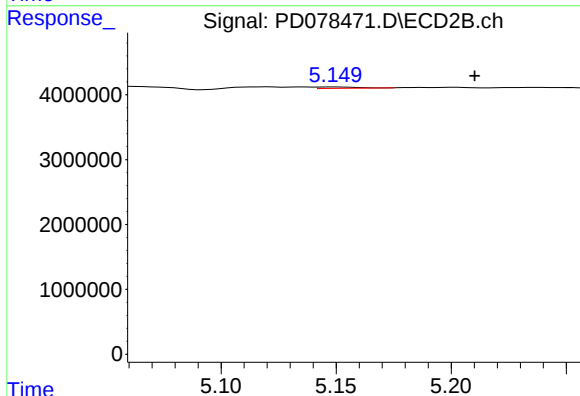


#12 4,4'-DDE

R.T.: 5.150 min
Delta R.T.: -0.060 min
Response: 231958
Conc: 0.11 ng/ml

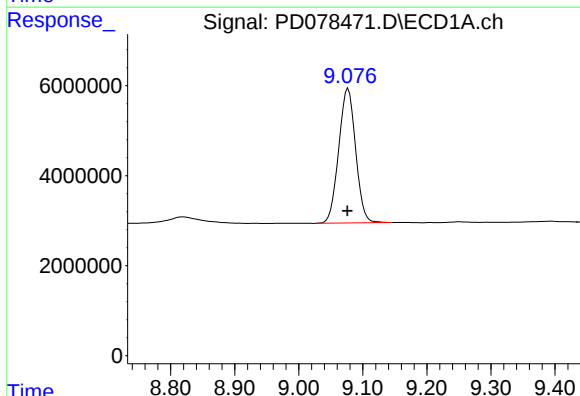

#27 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.001 min
Response: 54720233
Conc: 16.93 ng/ml

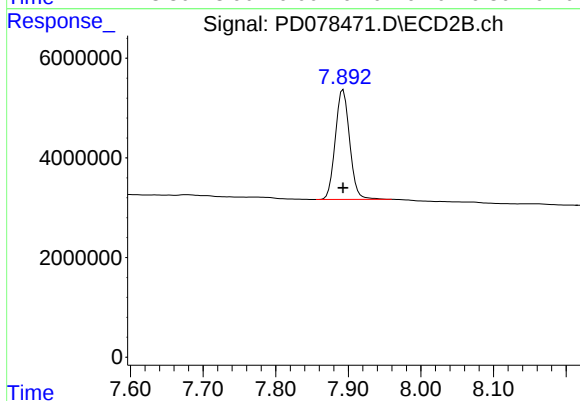

#27 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 30267046
Conc: 16.35 ng/ml