

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 16:22
 Operator : AR\AJ
 Sample : PB155923BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:37:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	48169157	31932520	19.617	19.329
27)	SA Decachlor...	9.078	7.893	67010107	37803120	20.730	20.420
Target Compounds							
3)	MA gamma-BHC...	0.000	3.597	0	29812	N.D.	<MDL
5)	MB Aldrin	0.000	4.196	0	22045	N.D.	<MDL
8)	B Heptachlo...	0.000	4.747f	0	53043	N.D.	<MDL
9)	A Endosulfan I	0.000	5.071	0	196483	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.071f	0	196483	N.D.	<MDL
12)	B 4,4'-DDE	0.000	5.146f	0	101129	N.D.	<MDL
14)	MA Endrin	0.000	5.549f	0	115529	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 16:22
Operator : AR\AJ
Sample : PB155923BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:37:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

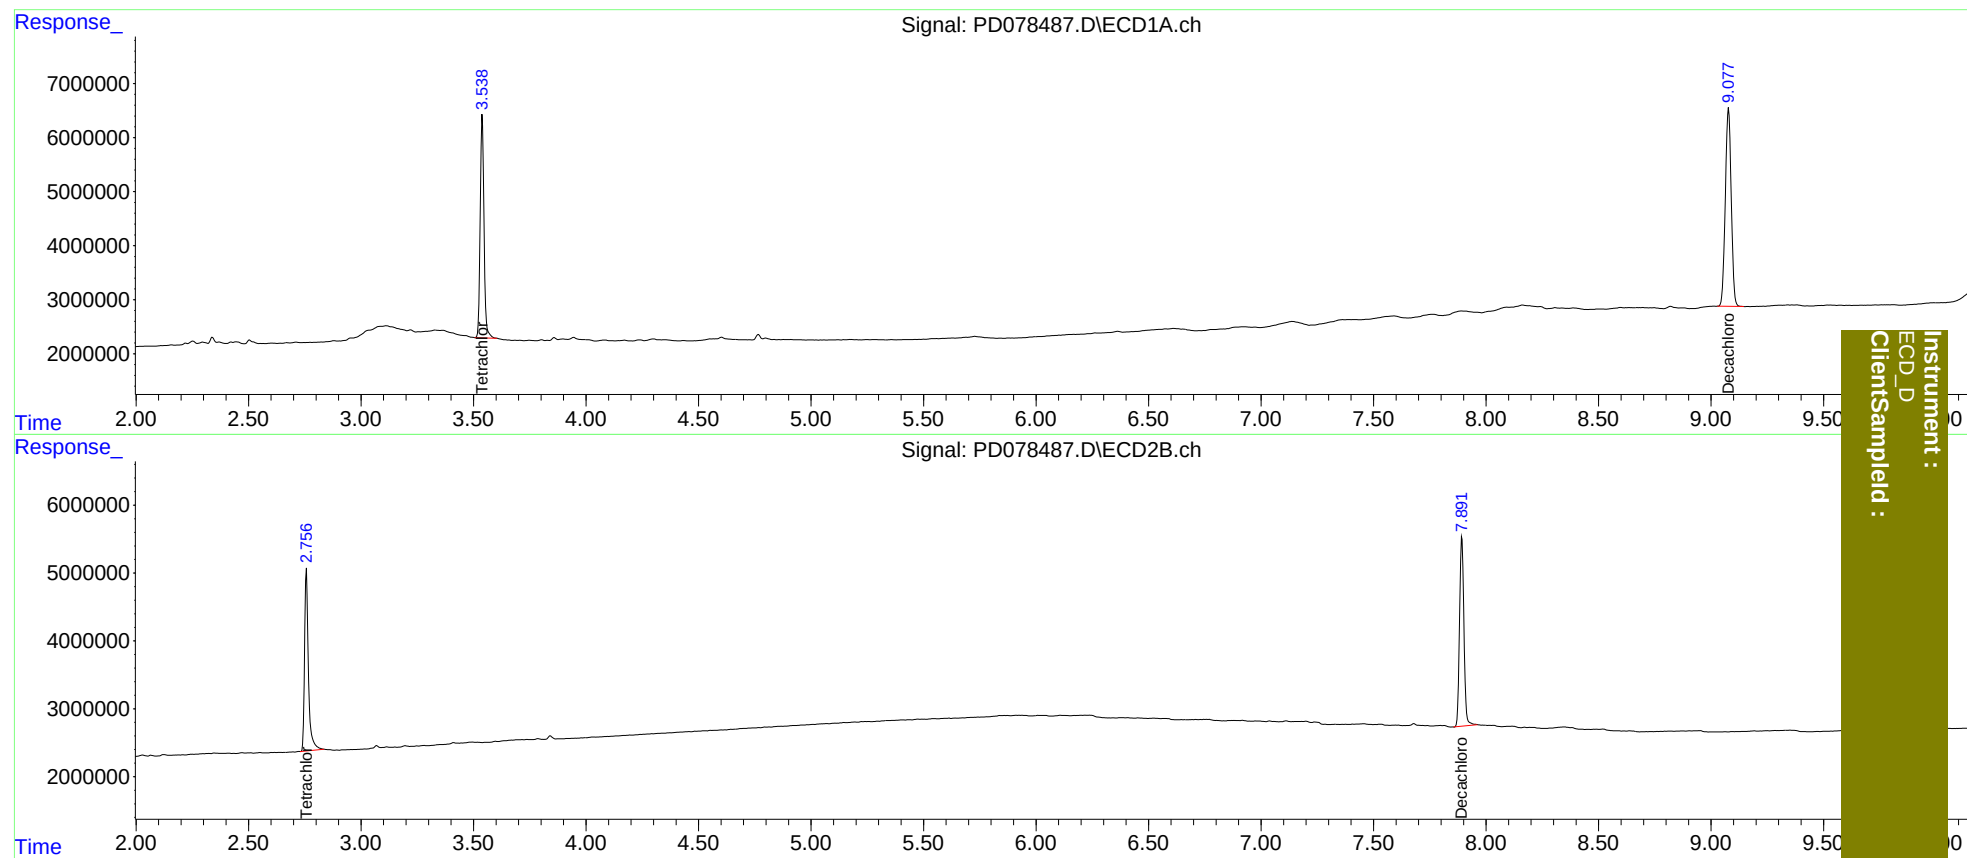


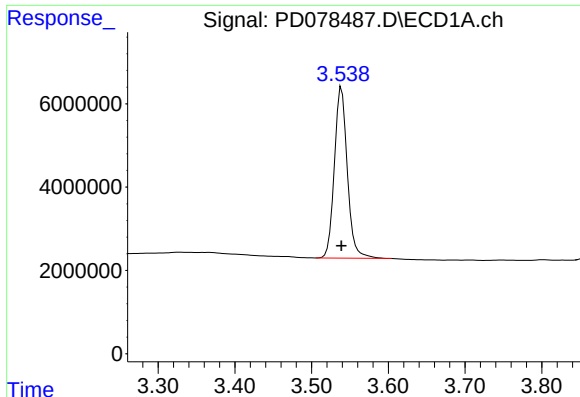

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 48169157
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

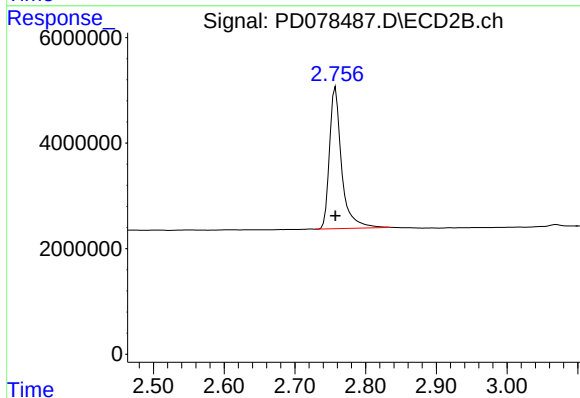


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 31932520
Conc: 19.33 ng/ml

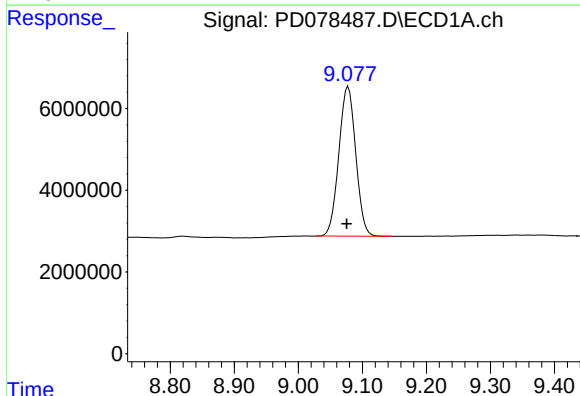

#27 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.002 min
Response: 67010107
Conc: 20.73 ng/ml

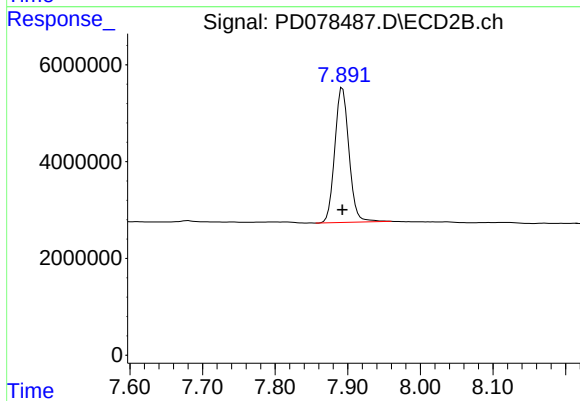

#27 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 37803120
Conc: 20.42 ng/ml